

Systematic Review

Validity, reliability, and clinical usefulness of instruments for measuring thoracic kyphosis: a systematic review and meta-analysis

Ana Paula Flôr Alves Nepomuceno^{a,d} , Ana Carolina Cury^a, Larissa Santos Pinto Pinheiro^{a,b}, George Schayer Sabino^{a,c}, Thales Rezende Souza^a , Sérgio Teixeira Fonseca^a, Juliana Melo Ocarino^{a,b} , Renan Alves Resende^{a,b,*} 

^a Department of Physical Therapy, Graduate Program in Rehabilitation Sciences, School of Physical Education, Physiotherapy and Occupational Therapy, Universidade Federal de Minas Gerais, Belo Horizonte, MG, Brazil

^b Sports Training Center, Universidade Federal de Minas Gerais, Belo Horizonte, Brazil

^c Institute of Innovation and Technological Incorporation Medical Sciences, Faculdade Ciências Médicas, Belo Horizonte, Minas Gerais, Brazil

^d Sarah Network of Rehabilitation Hospitals, Belo Horizonte, MG, Brazil



ARTICLE INFO

Keywords:

Measurement

Posture

Reliability

Thoracic kyphosis

Validity

ABSTRACT

Introduction: Thoracic hyperkyphosis is related to different health conditions, requiring precise evaluation in clinical settings. Several instruments have been proposed for assessing thoracic kyphosis, and previous studies have investigated their reliability and validity.

Aims: Systematically review studies evaluating the validity and reliability of instruments designed to measure thoracic kyphosis and classify their clinical utility.

Methods: MEDLINE and EMBASE (via Ovid) databases were used to search studies published until December 2023, and additional searches were conducted in Google Scholar and by hand search. Studies that analyzed the reliability and validity of noninvasive instruments for measuring thoracic kyphosis, regardless of population, study design, and language, were included. Two independent reviewers analyzed the titles, abstracts, and full text and assessed the methodological quality. Clinical utility was assessed using a 10-point scale.

Results: Seventy-two studies were included, and 15 instruments had their measurement properties explored: seven were grouped in a meta-analysis for validity, seven for intra-rater reliability, and six for inter-rater reliability. Despite the heterogeneity of estimated data, they presented a strong to moderate correlation with the gold standard and excellent intra- and inter-rater reliability. The instruments most frequently studied were the Flexicurve Angle and the Analog Inclinator.

Conclusion: The meta-analysis demonstrated that the Analog Inclinator, Flexicurve Angle and Index, Photogrammetry, Smartphone applications, and Spinal Mouse were valid and reliable for assessing thoracic kyphosis. Also, the utility analysis suggested that the Analog Inclinator, Flexicurve Angle, and Smartphone applications are recommended for clinical settings.

Introduction

In clinical practice, physical therapists usually assess thoracic kyphosis using visual inspection.¹ This method may not accurately quantify changes associated with different health conditions, aging, and treatments. Previous studies demonstrated that thoracic hyperkyphosis is associated with the presence of neck and low back pain,²⁻⁴ reduced lung function,⁵ impaired performance during gait,⁶ and increased risk of falls and mortality.⁷⁻⁸ Furthermore, evidence suggests that corrective

exercises for thoracic hyperkyphosis can improve posture and balance in patients with kyphosis angles greater than 40°. ⁹⁻¹⁰ Therefore, assessing thoracic kyphosis in clinical settings is essential for understanding, monitoring, and planning treatment for patients with several health conditions.

The Modified Cobb angle is the gold standard for measuring thoracic kyphosis using radiography (X-ray) due to its proven accuracy in assessing spinal curvature, its ability to provide detailed images of bone structures, and its widespread use in clinical practice as a reliable tool

* Correspondence author at. Universidade Federal de Minas Gerais (UFMG), Avenida Antônio Carlos, 6627 Belo Horizonte, 31270010, MG, Brazil.

E-mail address: renan.aresende@gmail.com (R.A. Resende).

<https://doi.org/10.1016/j.bjpt.2025.101246>

Received 3 July 2024; Received in revised form 2 December 2024; Accepted 7 July 2025

Available online 7 August 2025

1413-3555/© 2025 Associação Brasileira de Pesquisa e Pós-Graduação em Fisioterapia. Published by Elsevier España, S.L.U. All rights are reserved, including those for text and data mining, AI training, and similar technologies.

for diagnosis.¹¹ However, this assessment has limitations, including the time required for X-ray acquisition and interpretation, high costs, limited equipment portability, and radiation exposure, which is particularly concerning for repeated assessments in pediatric populations and young individuals.¹² Previous studies observed that the normal range of thoracic kyphosis varies between 20° and 40° in adolescents and younger adults.^{11,13} Although the definition of pathological hyperkyphosis is not a consensus, an angle greater than 50° has been adopted for this diagnosis.¹⁴ On the other hand, kyphosis angles < 20° characterize hypokyphosis.¹⁵

Using portable, easy-to-use, low-cost instruments may be beneficial for assessing thoracic kyphosis in clinical settings as it allows a quick, comfortable, and accurate measurement. However, instruments should not be used without evidence about their measurement properties.¹⁶ Previous studies investigated the validity and reliability of several instruments developed to assess thoracic kyphosis.^{12,17–39} Given the variety of instruments, clinicians must use instruments that ensure the proper assessment of thoracic kyphosis in clinical settings. This assessment enables monitoring to prevent or minimize negative consequences and evaluate treatment effectiveness related to thoracic hyper and hypokyphosis.

In 2014, a systematic review included 28 studies published up to October 2012 about the validity and reliability of non-radiographic methods for assessing thoracic kyphosis.⁴⁰ Findings showed that the validity of methods varied from low to very high, with reliability levels ranging from high to very high; however, no meta-analysis was performed. Despite the substantial number of studies included in this review, several additional studies investigated the measurement properties of instruments that assess thoracic kyphosis from October 2012 to the present day.

Therefore, this systematic review performed a meta-analysis of studies that assessed the validity and intra- and inter-rater reliability of clinical instruments proposed to quantify thoracic kyphosis in any population and classified the instruments according to their clinical utility.

Methods

Protocol

This systematic review was conducted in accordance with the Preferred Reporting Items for Systematic Reviews and Meta-Analyses (PRISMA) guidelines⁴¹ and is registered in PROSPERO (CRD42019124956).

Search strategy

The search was initially conducted in March 2019 and updated in December 2023 in MEDLINE, EMBASE (via Ovid), and Google Scholar databases. In addition, the reference lists of previous reviews and included studies were also hand-searched. The search terms were related to thoracic kyphosis, thoracic posture, measurement properties (validity and reliability), and clinical instruments. The search strategy is detailed in Supplementary material 1.

Eligibility criteria

The ideal instrument should be portable, precise, accurate, and affordable, thus allowing quick and safe assessment of thoracic kyphosis in clinical settings.⁴² Studies that assessed the validity or intra- or inter-rater reliability of clinical instruments proposed for measuring thoracic kyphosis were included. No language, publication date, sample characteristics, or study design restrictions were applied. Moreover, for the validity studies, instruments should be compared to an X-ray examination (gold standard) to be included. Studies that did not analyze the orthostatic posture of the thoracic region in the sagittal plane were

excluded.

Study selection and data extraction

Two independent reviewers (APFAN and ACC) analyzed titles and abstracts; ineligible studies were excluded. Then, two reviewers (APFAN and ACC) performed the full-text analysis. A third reviewer (RAR) resolved any disagreements in these steps. Data extraction was performed by one reviewer (APFAN). Descriptive information included sample characteristics (e.g., number of participants, sex, age, health condition, height, and body mass) and the instrument used to assess thoracic kyphosis. When applicable, the values of concurrent validity (Pearson correlation – r), intra- and inter-rater reliability (intraclass correlation coefficient – ICC), standard error of measurement (SEM), minimum detectable change (MDC), and Bland-Altman agreement analysis [(Mean Difference (MD) $\pm$ Standard Deviation (SD) and limits of agreement (LA)] were extracted. When two references for intra-rater reliabilities were reported, the ICC value of the most experienced rater or the higher value was chosen.

In addition, when studies measured the erect and relaxed thoracic kyphosis, only the value of the relaxed posture was considered, as it was adopted in most studies. Data were analyzed independently in the meta-analysis when the same study evaluated two or more instruments and different populations. Authors of validity studies that did not present the Pearson correlation and reliability studies that did not present the ICC value and 95 % confidence interval (95 % CI) were contacted by email to request data.

Methodological quality assessment


Two independent reviewers (APFAN and ACC) evaluated the methodological quality of the studies using the critical appraisal tool (CAT) checklist by Brink and Louw.⁴³ A third reviewer (RAR) resolved disagreements regarding the scoring of the studies. The CAT was structured to critically evaluate the measurement properties of instruments used in clinical settings and encompasses 13 items related to characteristics of population and evaluators, risk of bias, and methodological quality of the studies. Following the procedures adopted in previous systematic reviews, studies scoring above 60 % were considered to have high methodological quality.^{40,44–45} In this assessment, Kappa showed an overall agreement of 0.89 between the two independent reviewers (APFAN and ACC).

Data analysis

Concurrent validity and intra- and inter-rater reliabilities of individual studies were grouped using a random effects model and analyzed using Comprehensive Meta-analysis software (version 4.0). I^2 statistic was used to evaluate heterogeneity between studies.⁴⁶ Findings of individual studies and combined estimates were presented in a forest plot with a 95 % CI.

The concurrent validity was classified as very low ($r < 0.25$), low to reasonable ($0.25 \leq r < 0.50$), moderate to good ($0.50 \leq r < 0.75$), and strong ($r \geq 0.75$).¹⁶ In addition, we also reported Bland Altman's limits of agreement.¹⁶ The intra- and inter-rater reliabilities were classified as low ($ICC < 0.40$), good to moderate ($0.40 \leq ICC < 0.74$), and excellent ($ICC \geq 0.75$).⁴⁷

To be recommended for clinical use, an instrument must meet rigorous criteria, including validity ($r > 0.80$), reliability ($ICC > 0.80$), sensitivity (MDC), and a score of 9 or higher on a 10-point clinical utility scale. This scale evaluates factors such as portability, cost, evaluation time, measurement analysis, and interpretation. Specifically, cost is scored as follows: < £100 scores 3, £100 - £500 scores 2, £500 - £1000 scores 1, and > £1000 or unknown scores 0. Evaluation time is evaluated based on duration: <10 min scores 3, 10–30 min scores 2, 30–60 min scores 1, and >1 h scores 0. The necessity of specialized equipment or

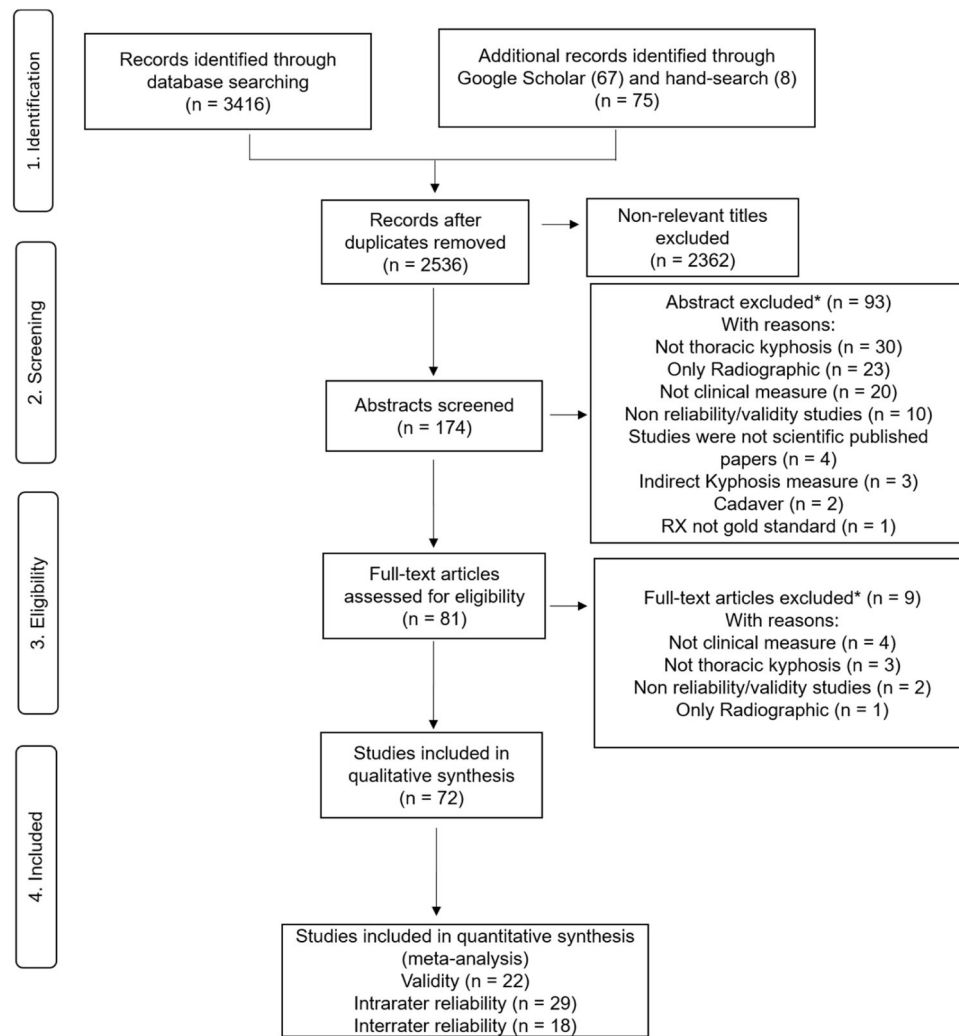

*Abstracts and potentially relevant full-texts could be excluded due to more than one inclusion criterion.

Fig. 1. - PRISMA flow-chart of studies through the review.

professional training is also considered, with “No” scoring 2, “Yes, but only simple, easy to use equipment, which does not need specialist training” scoring 1, and “Yes” or “Unknown” scoring 0. Finally, portability is evaluated as follows: “Yes, easily (e.g., can fit in a pocket)” scores 2, “Yes, but requires a briefcase or trolley” scores 1, and “No or very difficult” scores 0.^{48–49}

Results

Flow of studies

The search strategy identified 2536 titles after excluding duplicates. After screening titles and abstracts, 81 studies were included for full-text review. Four studies were excluded because they did not use clinical instruments, three for not measuring thoracic kyphosis, one because they were not validity or reliability studies, and one because thoracic kyphosis was measured only on the X-ray films. The studies excluded by full-text are listed in a table in the Supplementary material 2. Therefore, 72 studies were included. The review flowchart is presented in Fig. 1.

Characteristics of the included studies

The characteristics of the studies are described in Tables 1 and 2.

Fifteen instruments were identified: Analog Inclinator, Archometer, Baseline® Body Level/ Scoliosis meter, Debrunner Kyphometer, Electrogoniometer, Digital Inclinator, Dual Digital Inclinator, Flexicurve (Angle and Index), Kypholordometer, Microsoft Kinect Sensor, Photogrammetry, Smartphone app, Spinal Mouse, Spinal Pantograph, and Spinal Wheel. Among the included studies, 31 verified the concurrent validity by comparing the instrument with an X-ray in the sagittal plane,^{12,17,19–20,23–24,29,31,33–34,50–70} 57 evaluated the intra-rater reliability,^{12,17–18,20–28,30–32, 35–39, 42, 50–52,54–57,63–65,67–69,71–94} and 40 the inter-rater reliability.^{12,17,20–24,27–28, 30, 32–33, 35,51,54–57,64–65, 68–74,78–80,82–83,87–91,93,95–96}

The studies sample size ranged from 11 to 139 participants. Regarding the sample of the studies, 33 (45.83 %) evaluated healthy individuals, 20 (27.77 %) included patients with kyphosis or scoliosis, eight (11.11 %) included patients with musculoskeletal pain in different body regions, five (6.94 %) included patients with osteoporosis or reduced bone mass, five (6.94 %) included individuals who had been referred for a thoracic spine X-ray, three (4.16 %) evaluated athletes, two (2.77 %) evaluated patients with Parkinson’s, one (1.38 %) evaluated individuals with some orthopedic condition and one (1.38 %) did not characterize the sample. Regarding the age group, 14 studies (19.44 %) evaluated individuals aged ≥ 60 years, 40 (55.94 %) evaluated adults aged between 18 and 60 years, and 20 (27.77 %) evaluated children and

Table 1
Characteristics of the included validity studies.

Authors and year of the study	Instrument	Study Population	Validity levels
Azadinia et al. 2021 ⁵⁰	Photogrammetry (Digimizer Image Analysis Software version 5.3.4 -MedCalc Software; BVBA, Ostend, Belgium)	$n = 50$ Mean age $\pm$ SD = 13.72 ± 1.85 years; BMI (kg/m^2) 19.37 ± 2.87 Sex (M/F) 26/24 Adolescents with hyperkyphosis	$r = 0.94$ $BA = 3.91^\circ$ (MD); SD = NR $LA = 10.2^\circ$ to -2.4°
Azadinia et al. 2014 ⁵¹	Dual Digital inclinometer (DDI) Flexicurve Angle (FA)	$n = 81$ Mean age $\pm$ SD = 14.69 ± 4.11 years (range 10 - 30 years); height (cm) 157 ± 13.5 ; mass (kg) 50.7 ± 15.3 BMI _C (kg/m^2) 20 Sex (M/F) 26/55 Patients with Hyperkyphosis $n = 21$ Mean age $\pm$ SD = 65.76 ± 4.6 years (range 50 - 80 years); height (cm) 156.8 ± 5.7 ; mass(kg) 66.48 ± 8.93 BMI _C (kg/m^2) 26 Sex (M/F) 3/18 Patients with Hyperkyphosis	$r = \text{NR}$ $\text{ICC}_{\text{DDIRX}} = 0.89$ $BA_{\text{DDI}} = 4.85^\circ$ (SD) MD = NR; LA = NR $\text{ICC}_{\text{FARX}} = 0.51$ $BA_{\text{FA}} = 9.30^\circ$ (SD) MD = NR; LA = NR $r = \text{NR}$ $\text{ICC}_{\text{DDIRX}} = 0.81$ $BA_{\text{DDI}} = 4.93^\circ$ (SD) MD = NR; LA = NR $\text{ICC}_{\text{FARX}} = 0.50$ $BA_{\text{FA}} = 8.03^\circ$ (SD) MD = NR; LA = NR $r = 0.78$ $BA = \text{NR}$
Barauna et al. 2005 ⁵²	Kypholordometer	$n = 30$ Mean age $\pm$ SD = 39 ± 15.8 years BMI = NR Sex (M/F) NR Scheuermann's Disease ($n = 3$) Postural kyphosis ($n = 25$) Ankylosing Spondylitis ($n = 2$)	$r = 0.78$ $BA = \text{NR}$
Barrett et al. 2017 ⁵³	Analog Inclinometer (AI) Flexicurve Angle (FA)	$n = 11$ Mean age $\pm$ SD = 40.9 ± 20.1 years BMI (kg/m^2) 24.4 ± 5.4 Sex (M/F) 7/4 Patients with pain ($n = 6$ low back pain; $n = 4$ with thoracic pain; $n = 1$ with inter-scapular pain)	$r_{\text{AIRX}} = 0.86$ $BA_{\text{AI}} = 4.8^\circ \pm 8.9^\circ$ (MD $\pm$ SD) LA = 22.28° to -12.64° $r_{\text{FARX}} = 0.96$ $BA_{\text{FA}} = 20.2^\circ \pm 6.1^\circ$ (MD $\pm$ SD); LA = 32.27° to 8.29° $r = 0.93$ $BA = \text{NR}$
Büyükturan et al. 2018 ⁵⁴	Spinal Mouse	$n = 46$ Mean age $\pm$ SD = 68.12 ± 2.67 years BMI (kg/m^2) 29.45 ± 4.67 Sex (M/F) 17/29 Healthy older individuals	$r = 0.93$ $BA = \text{NR}$

Table 1 (continued)

Authors and year of the study	Instrument	Study Population	Validity levels
Chaise et al. 2011 ²⁴	Arcometer	$n = 52$ Mean age $\pm$ SD = 53.7 ± 14.9 years BMI (kg/m^2) 26.1 ± 4.4 Sex (M/F) NR Persons with prescription for an X-ray	$r = 0.94$ $BA = -1.4^\circ \pm 6.06^\circ$ (MD $\pm$ SD); LA = 10.53° to -13.24°
de Oliveira et al. 2012 ⁵⁵	Flexicurve Angle	$n = 47$ Mean age $\pm$ SD = 44.9 ± 19.4 years BMI (kg/m^2) 27.5 ± 5 Sex (M/F) Both sex Persons with prescription for an X-ray	$r = 0.70$ $BA = 0.8^\circ \pm 8.0^\circ$ (MD $\pm$ SD); LA = 17.0° to -15.3°
D'Oswaldo et al. 1997 ⁵⁶	Arcometer	$n = 32$ Mean age 15.5 years BMI = NR Sex (M/F) 9/23 Patients with kyphosis and scoliosis, and for postural rehabilitation	$r = 0.98$ $BA = \text{NR}$
Faramarzi et al. 2020 ⁵⁷	Smartphone app (Goniometer-Pro app)	$n = 31$ Mean age $\pm$ SD = 25.09 ± 4.02 years; BMI (kg/m^2) 22.07 ± 1.44 Sex (M/F) NR Persons with prescription for an X-ray	$r = 0.81$ $BA = 1.79^\circ \pm 5.40^\circ$ (MD $\pm$ SD) LA = NR
Fortin et al. 2010 ³⁴	Photogrammetry (Fringes Acquisition and Processing Software - InSpec Inc., Montreal, Canada)	$n = 70$ (validity $n = 40$) Mean age $\pm$ SD = 15.7 ± 2.5 years BM (kg) 51.9 ± 9.3 Height (cm) 161 ± 9.5 BMI _C (kg/m^2) 20 Sex (M/F) 10/60 Children with Scoliosis	$r = -0.77$ $BA = \text{NR}$
Giglio and Volpon, 2007 ⁵⁸	Spinal Pantograph	$n = 718$ (validity = 20) Mean age 11.45 years BMI = NR Sex (M/F) 350/368 Normal subjects	$r = 0.70$ $BA = \text{NR}$
Gravina et al. 2012 ⁵⁹	Analog Inclinometer	$n = 128$ Mean age 12.7 years BMI = NR Sex (M/F) Both sex Children/adolescents idiopathic scoliosis. Scheuermann or postural kyphosis	$r = 0.89$ $BA = -0.3^\circ$ (MD) SD = NR LA = 17.0° to -16°
Greendale et al. 2011 ¹²	Debrunner Kyphometer (DB) Flexicurve angle (FA) Flexicurve index (FI)	$n = 113$ Mean age $\pm$ SD = 75.3 ± 7.5 years BMI (kg/m^2) 26.5 ± 4.5 Sex (M/F) 80.5 % were women Persons with Kyphosis $> 40^\circ$	$r_{\text{DBRX}} = 0.62$ $BA_{\text{DK}} = 10.96^\circ$ (SD); MD = NR; LA = NR $r_{\text{FARX}} = 0.68$ $BA_{\text{FA}} = 10.24^\circ$ (SD); MD = NR; LA = NR $r_{\text{FIRX}} = 0.68$ $BA_{\text{FI}} = 11.26^\circ$

(continued on next page)

Table 1 (continued)

Authors and year of the study	Instrument	Study Population	Validity levels
Grindle et al. 2020 ⁶⁰	Flexicurve angle (FA)	$n = 40$ Mean age 55.9 ± 24.71 years. BMI (kg/m ²) 24.7 ± 3.3 Sex (M/F) 18/22 Adult volunteers with hyperkyphosis	(SD); MD = NR; LA = NR $r = \text{NR}$ ICC = 0.55 (0.29 – 0.73) BA = NR
Hannink et al. 2022 ⁶¹	Dual Digital inclinometer (DDI) Flexicurve index (FI) Microsoft Kinect Sensor index (MKS)	$n = 29$ Mean age 56.9 ± 18.2 years BMI (kg/m ²) 24.7 ± 4.3 Sex (M/F) 6/23 Persons with spinal conditions	$r_{\text{DDIRX}} = 0.67$ $BA_{\text{DDI}} = 3.51^\circ$ (MD); SD = NR; LA = NR $r_{\text{FIRX}} = 0.54$ $BA_{\text{FI}} = 0.079^\circ$ (MD); SD = NR; LA = NR $r_{\text{MKSIX}} = 0.70$ $BA_{\text{MKS}} = 0.004^\circ$ (MD); SD = NR; LA = NR
Hunter et al. 2018 ⁶²	Analog Inclinometer	$n = 78$ - 39 with shoulder impingement syndrome Mean age ± SD 57.1 ± 11.1 years; BMI (kg/m ²) 29.3 ± 5.32 Sex (M/F) 20/19 - 39 no shoulder pain Mean age ± SD 55.7 ± 10.6 years; BMI (kg/m ²) 25.7 ± 3.53 Sex (M/F) 19/20	$r = 0.62$ BA = 2.45° ± 8.38° (MD ± SD); LA = 18.87° to -13.97°
Kado et al. 2006 ¹⁹	Debrunner Kyphometer	$n = 120$ Mean age ± SD 68.6 ± 5.9 years BMI = NR Sex (M/F) 0/120 Women with low bone mineral density (0.68 g/cm ²)	$r = \text{NR}$ BA = NR ICC = 0.68
Korovessis et al. 2001 ²⁰	Debrunner Kyphometer	$n = 90$ Mean age ± SD 15 ± 2.6 years BMI = NR Sex (M/F) 44/46 Adolescents with round back or poor sagittal back appearance	$r = 0.75$ BA = NR
Perriman et al. 2010 ³¹	Electrogoniometer	$n = 12$ Mean age 68.1 (50 - 80) years. BM (kg) 75.8 (62 - 94) Height (cm) 171.2 (160–190); BMI _C (kg/m ²) 25 Sex (M/F) 6/6 Healthy older individuals	$r = 0.87$ BA = NR
Prowse et al. 2018 ³³	Baseline® Body Level/ Scoliosis meter	$n = 31$ Mean age ± SD 13.6	$r = -0.32$ BA = NR

Table 1 (continued)

		± 0.6 years BMI = NR Sex (M/F) 4/27 Adolescent with scoliosis	
Sangtarash et al. 2014 ⁶³	Dual Digital Inclinometer	$n = 20$ Mean age ± SD 57.20 ± 7.67 years BMI (kg/m ²) 27.75 ± 4.47 Sex (M/F) 0/20 Women with back pain	$r = \text{NR}$ ICC = 0.86 BA = -1.55° ± 6.88° (MD ± SD) LA = 12.26° to -15.21°
Sedrez et al. 2014 ²³	Arcometer	$n = 40$ Mean age ± SD 10.7 ± 2.7 years BM (kg) 38.7 ± 13.1 Height(m) 1.39 ± 0.17 BMI _C (kg/m ²) 20 Sex (M/F) 25/15 Children (status not reported)	$r = 0.40$ BA = NR
Schmidt et al. 2022 ⁶⁴	Analog Inclinometer	$n = 16$ Group 1 Risser 1 or 2 Mean age ± SD 12.3 ± 1.0 years BMI (kg/m ²) 20.3 ± 3.3 Sex (M/F) NR Adolescent with idiopathic scoliosis	$r_{\text{group1}} = 0.84$ BA = NR $r_{\text{group2}} = 0.75$ BA = NR
Sharifnezhad et al. 2021 ⁶⁵	Photogrammetry (Kinovea software)	$n = 23$ Group 2 Risser 3 or 4 Mean age ± SD 15.0 ± 1.7 years BMI (kg/m ²) 24.1 ± 4.9 Sex (M/F) NR Adolescent with idiopathic scoliosis	$r = 0.48$ BA = NR
Spencer et al. 2019 ⁶⁶	Flexicurve Angle	$n = 117$ Mean age ± SD 61.4 ± 7.0 years BMI (kg/m ²) 29.0 ± 5.5 Sex (M/F) 0/117 Postmenopausal women with upper back pain	$r = 0.64$ BA = -2.48° (MD) SD = NR LA = 14.92° to -19.88°
Tabard-Fougere et al. 2019 ⁶⁷	Analog Inclinometer	$n = 51$ Mean age ± SD 13.5 ± 2.0 years BMI (kg m ²) 18.9 ± 2.8 Sex (M/F) 19/32 Adolescent with idiopathic scoliosis	$r = 0.73$ BA = NR
Teixeira et al. 2007 ⁶⁸	Flexicurve Angle	$n = 56$ Mean age ± SD 66.7 ± 9.37 years	$r = \text{NR}$ BA = NR ICC = 0.90

(continued on next page)

Table 1 (continued)

Authors and year of the study	Instrument	Study Population	Validity levels
Todd et al. 2015 ⁶⁹	Debrunner Kyphometer	BMI = NR Sex (M/F) 21 /35 Healthy older individuals n = 92 Mean age ± SD 17.7 ± 1.39 years BMI (kg/m ²) 22.9 ± 3.27 Young athletic elite alpine skiers (n = 75) Sex (M/F) 30/35 Non-athletic population (n = 27) Sex (M/F) 9/18	r = 0.60 BA = 4.5° (MD); SD = NR LA = 7.7° to -16.8°
Tran et al. 2016 ⁷⁰	Debrunner Kyphometer (DK) Flexicurve Index (FI)	n = 72 (FI); n = 71 (DK) Mean age ± SD 77.8 ± 7.1 years BMI (kg/m ²) 25.3 ± 4.6 Sex (M/F) 20/52 Persons recruited from Community with thoracic kyphosis	r _{DBRX} = 0.65 BA = NR r _{FIRX} = 0.68 BA = NR
Willner Stig, 1981 ¹⁷	Spinal Pantograph	n = 71 (n = 15 cases with a structural scoliosis of <30°; n = 41 cases without any visible spinal disorder on X-ray who served as "controls"; n = 15 cases with Scheuermann's disease) Mean age ± SD = NR BMI = NR Sex (M/F) = NR Teenagers with or without visible spinal disorder	r = 0.97 BA = NR
Yousefi et al. 2012 ²⁹	Flexicurve Angle (FA) Spinal Mouse (SM) Photogrammetry (pH)	n = 20 Mean age ± SD 26 ± 2 years BM (kg) 72 ± 2.5 Height (cm) 169 ± 5.5 BMI _C (kg/m ²) 25 Sex (M/F) 20/0 Student volunteers	r _{FARX} = 0.87 BA = NR r _{SMRX} = 0.76 BA = NR r _{PHRX} = 0.89 BA = NR

Note. NR, Not reported; BMI, Body Mass Index; BMI_C, Body Mass Index calculated; SD, Standard deviation; BA, Bland-Altman analysis; BA_{AI}, BA Analog Inclinometer; BA_{DDI}, BA Dual Digital Inclinometer; BA_{FA}, BA Flexicurve Angle; BA_{FI}, BA Flexicurve Index; BA_{DB}, Debrunner Kyphometer; LM, Limits of agreement; MD, Mean difference; ICC, Intraclass Correlation Coefficient; ICC_{DDIRX}, Intraclass Correlation Coefficient Dual Digital Inclinometer x RX; ICC_{FARX}, Intraclass Correlation Coefficient Flexicurve Angle x RX; r, Correlation; r_{AIRX}, Correlation Analog Inclinometer x RX; r_{FIRX}, Correlation Flexicurve Index x RX; r_{FARX}, Correlation Flexicurve Angle x RX; r_{DKRX}, Correlation Debrunner's Kyphometer x RX; r_{DDIRX}, Correlation Dual Digital Inclinometer x RX; r_{MKSIX}, Correlation Microsoft Kinect Sensor x RX; r_{SMRX}, Correlation Spinal Mouse x RX; r_{PHRX}, Correlation Photogrammetry x RX.

adolescents. Regarding sex, 56 (77.77 %) studies included individuals of both sexes, nine (12.50 %) included only women, two (2.77 %) included only men, and five (6.94 %) studies did not report the sex of the individuals.

Between the studies that reported the type of orthostatic posture during the measurement of thoracic kyphosis, 43 (59.72 %) evaluated the relaxed orthostatic posture, 16 (22.22 %) the upright orthostatic posture, and 4 (5.55 %) evaluated both postures.

Methodological quality of included studies

The methodological quality is reported in Supplementary material 3. Of the 72 studies, 62 (86.11 %) had high quality. Regarding validity, of the 31 studies, 26 (83.87 %) had high methodological quality. Of the 58 intra-rater reliability studies, 50 (86.20 %) were of high quality and 33 (82.50 %) out of the 40 inter-rater reliability studies were of high quality. The CAT items with the worst scores were related to the lack of randomization of evaluators or individuals and the lack of information about the qualifications and experience of the raters, the rater blinding process, and the time interval between the measurement by the instrument and the gold standard.

Validity

A total of 13 instruments had concurrent validity assessed in 31 studies (Table 1). The most investigated were the Analog Inclinometer and Flexicurve Angle. On the other hand, the validity of the Digital Inclinometer and Spinal Wheel was not investigated. The Baseline® Level/Scoliosis meter (r = 0.32),³³ Kipholordometer (r = 0.78),⁵² Electrogoniometer (r = 0.87),³¹ Dual Digital Inclinometer (r = 0.67),⁶¹ Microsoft Kinect Sensor (r = 0.70),⁶¹ and the Smartphone app (r = 0.81)⁵⁷ had the validity tested in only one study; thus, they were not included in the meta-analysis. Seven instruments presented the correlation coefficient with the X-ray examination reported by at least two studies; therefore, they were grouped into seven meta-analyses, one for each instrument (Fig. 2). The meta-analysis demonstrated that the Analog Inclinometer, Arcometer, Flexicurve Angle, Photogrammetry, Spinal Mouse and Spinal Pantograph presented strong concurrent validity with the X-ray. The Debrunner Kyphometer and Flexicurve Index demonstrated moderate levels of concurrent validity with the X-ray (Fig. 2). Bland-Altman analysis was described for nine instruments and is presented as the mean difference between measurements (Table 1).

Intra-rater reliability

Fourteen instruments had their intra-rater reliability assessed in 55 studies (Table 2); the Analog Inclinometer, Flexicurve Angle, and Photogrammetry were the most investigated. Seven instruments had the 95 % CI of the ICC reported by at least two studies and were grouped into seven metanalyses, one for each instrument. The following instruments demonstrated an excellent level of intra-rater reliability: Analog, Digital Inclinometer, Flexicurve Angle, Flexicurve Index, Photogrammetry, Microsoft Kinect Sensor, Smartphone app, and Spinal Mouse (Fig. 3). This analysis was not performed in studies that used the Baseline ® Level/Scoliosis meter.³³ The Kipholordometer⁵² and Spinal Pantograph¹⁷ instruments did not have the ICC reported. The Electrogoniometer (ICC = 0.90)³¹ and Spinal Wheel (ICC = 0.98),³² evaluated in only one study each, showed excellent intra-rater reliability. The Arcometer was evaluated in three studies: one did not report the ICC,⁵⁶ and the other two demonstrated levels of intra-rater reliability ranging from good to excellent (0.50 to 0.99) but did not report the 95 % CI of the ICC²³⁻²⁴; therefore, they were not included in the meta-analysis. The Debrunner Kyphometer^{12,20-21,69,84} and the Dual Digital Inclinometer^{51,63} were evaluated in five and two studies, respectively, and demonstrated excellent levels of intra-rater reliability. However, they also did not present the 95 % CI of the ICC and were not grouped in the meta-analysis. The MDC and SEM were reported for six and eight instruments, respectively (Table 2).

Inter-rater reliability

Twelve instruments had their inter-rater reliability assessed by 40 studies (Table 2); the Flexicurve Angle, the Debrunner Kyphometer, and the Analog Inclinometer were the most investigated. Six of these 12 instruments had ICC and 95 % CI of the ICC data reported by at least two

Table 2
Characteristics of the included reliability studies.

Authors and year of the study	Instrument	Study Population	Intrarater and Interrater Reliability	SEM/MDC
Alderighi et al. 2016 ⁷¹	Analog Inclinator	$n = 34$ Mean age $\pm$ SD 19.17 (4.52 years) BMI (kg/m ²) 21.00 $\pm$ 2.60 Sex (M/F) 0/34 Heathy female football players (> 3 h/ week) $\geq$ 3 years (weekly sport hours mean 6.56)	ICC _{IAR} = 0.91 95 % CI (0.85 – 0.98) ICC _{IER} = 0.88 95 % CI (0.82 – 0.94)	SEM _{IAR} = 2.09° SEM _{IER} = 2.44° MDC _{IER} = 6.77°
Amatachaya et al. 2016 ⁷²	Flexicurve Angle	$n = 21$ Mean age $\pm$ SD 74.1 $\pm$ 7.6 years; BMI (kg/m ²) 21.6 $\pm$ 3.7 Sex (M/F) NR Older individuals with various degrees of structural kyphosis	ICC _{IAR} = 0.97 95 % CI (0.94 – 0.98) ICC _{IER} = 0.94 95 % CI (0.86 – 0.97)	SEM _{IAR} = 2.69° MDC _{IAR} = 7.43° SEM _{IER} = 3.65° MDC _{IER} = 10.08°
Azadinia et al. 2021 ⁵⁰	Photogrammetry Digimizer Image Analysis Software version 5.3.4 (MedCalc Software; BVBA, Ostend, Belgium)	$n = 40$ Mean age $\pm$ SD 13.57 $\pm$ 1.99 years; BMI (kg/m ²) 19.28 $\pm$ 2.76 Sex (M/F) 20/20 Adolescents with hyperkyphosis	ICC _{IAR} = 0.97 95 % CI (0.94 – 0.98)	SEM _{IAR} = 1.67° MDC _{IAR} = 4.62°
Azadinia et al. 2014 ⁵¹	Flexicurve Angle (FA) Dual Digital inclinometer (DDI)	$n = 81$ Mean age $\pm$ SD 14.69 $\pm$ 4.11 years (range 10 – 30); height (cm) 157 $\pm$ 13.5; mass (kg) 50.7 $\pm$ 15.3 BMI _C (kg/m ²) 20 Sex (M/F) 26/55 Patients with hyperkyphosis $n = 21$ Mean age $\pm$ SD 65.76 $\pm$ 4.6 years; height (cm) 156.8 $\pm$ 5.7; mass(kg) 66.48 $\pm$ 8.93 BMI _C (kg/m ²) 26 Sex (M/F) 3/18 Patients with hyperkyphosis	ICC _{IARFA} (10 – 30) = 0.87 ICC _{IERFA} (10 – 30) = 0.68 ICC _{IARDDI} (10 – 30) = 0.98 ICC _{IERDDI} (10 – 30) = 0.96 ICC _{IARFA} (50 – 80) = 0.86 ICC _{IERFA} (50 – 80) = 0.85 ICC _{IARDDI} (50 – 80) = 0.97 ICC _{IERDDI} (50 – 80) = 0.92	SEM = NR MDC = NR
Barrett et al. 2013 ⁷³	Analog Inclinator (AI) Flexicurve Angle (FA) Flexicurve Index (FI)	$n = 30$ intrarater reliability Mean age $\pm$ SD 45 $\pm$ 16 years BM (kg) 73.9 $\pm$ 11.1; Height (cm) 172.8 BMI _C (kg/m ²) 24 Sex (M/F) 18/12 $n = 12$ interrater reliability Mean age $\pm$ SD 49 $\pm$ 18 years. BM (kg) 74 $\pm$ 15; Height (cm) 172 $\pm$ 10 BMI _C (kg/m ²) 25 Sex (M/F) 5/7 Swimmers with or without shoulder pain (swimming at least 2 X week. Average Weekly swim distance (km) intrarater 9.9 (SD $\pm$ 14) and interrater 7 (SD $\pm$ 6)	ICC _{IARAI} = 0.92 95 % CI (0.84 – 0.96) ICC _{IERAI} = 0.90 95 % CI (0.68 – 0.97) ICC _{IARFA} = 0.94 95 % CI (0.88 – 0.97) ICC _{IERFA} = 0.86 95 % CI (0.51 – 0.96) ICC _{IARFI} = 0.94 95 % CI (0.88 – 0.97) ICC _{IERFI} = 0.86 95 % CI (0.51 – 0.96)	SEM _{IARAI} = NR SEM _{IERAI} = 2.2° MDC = NR SEM _{IARFA} = NR SEM _{IERFA} = 1° MDC = NR SEM _{IARFI} = NR SEM _{IERFI} = 0.4° MDC = NR
Barauna et al. 2005 ⁵²	Kypholordometer	$n = 30$ Mean age $\pm$ SD 39 $\pm$ 15.8 years BMI = NR Sex (M/F) both Scheuermann's Disease ($n = 3$) Postural kyphosis ($n = 25$) Ankylosing Spondylitis ($n = 2$)	ICC _{IAR} = NR	SEM = NR MDC = NR
Büyükturan et al. 2018 ⁵⁴	Spinal Mouse	$n = 46$ Mean age $\pm$ SD 68.12 $\pm$ 2.67 years BMI (kg/m ²) 29.45 $\pm$ 4.67 Sex (M/F) 17/29 Healthy elderly	ICC _{IAR} = 0.85 95 % CI (0.80 – 0.89) ICC _{IER} = 0.90 95 % CI (0.88 – 0.91)	SEM _{IAR} = 2.86° MDC = NR SEM _{IER} = 3.14° MDC = NR
Carvalho et al. 2019 ⁷⁴	Flexicurve Angle	$n = 21$ Mean age $\pm$ SD M: 22 $\pm$ 0.71 years; BM (kg) 78.25 $\pm$ 8.83; Height 1.82 $\pm$ 0.12 m BMI _C (kg/m ²) 23 F: 22 $\pm$ 1.41 years; BM (kg) 53 $\pm$ 2.88; Height 1.61 $\pm$ 0.04 m BMI _C (kg/m ²) 20 Sex (M/F) 4/17 Healthy and asymptomatic	ICC _{IAR} = 0.94 95 % CI (0.87 – 0.98) ICC _{IER} = 0.82 IC (0.60 – 0.93)	SEM _{IAR} = 2.3° MDC _{IAR} = 6.4° SEM _{IER} = NR MDC _{IER} = NR
Chaise et al. 2011 ²⁴	Arcometer	$n = 15$ intrarater reliability; $n = 30$ interrater reliability Mean age $\pm$ SD 53.7 $\pm$ 14.9 years BMI (kg/m ²) 26.1 $\pm$ 4.4 Sex (M/F) NR	ICC _{IAR} = 0.99 ICC _{IER} = 0.98	SEM = NR MDC = NR
Czaprowski et al. 2012 ²⁸	Digital inclinometer	$n = 30$ Mean age $\pm$ SD 23 $\pm$ 3.4 years BMI (kg/m ²) 21.4 $\pm$ 2.4 Sex (M/F) 5/25 Healthy subjects	ICC _{IAR} = NR ICC _{IER} = NR	SEM = NR MDC = NR

(continued on next page)

Table 2 (continued)

Authors and year of the study	Instrument	Study Population	Intrarater and Interrater Reliability	SEM/MDC
Demir et al. 2020 ⁷⁵	Spinal Mouse	$n = 28$ Mean age $\pm$ SD 16.29 ± 1.08 years BMI (kg/m^2) 21.14 ± 2.88 Sex (M/F) 0/28 Asymptomatic females	$\text{ICC}_{\text{IAR}} = 0.86$ 95 % CI (0.54 – 0.88)	SEM = NR MDC = NR
de Oliveira et al. 2012 ⁵⁵	Flexicurve Angle	$n = 15$ (intrarater reliability); $n = 47$ (interrater reliability) Mean age $\pm$ SD 44.9 ± 19.4 BMI (kg/m^2) 27.5 ± 5 Sex (M/F) both sex	$\text{ICC}_{\text{IAR}} = 0.82$ 95 % CI (0.56 – 0.93) $\text{ICC}_{\text{IER}} = 0.94$ 95 % CI (0.86 – 0.97)	$\text{SEM}_{\text{IAR}} = 1.3^\circ$ MDC = NR
Devaney et al. 2017 ⁷⁶	Analog Inclinator	Persons with prescription for an X-ray $n = 51$ intrarater reliability; Mean age $\pm$ SD 46.9 ± 20.2 years BMI = NR Sex (M/F) 25/26	$\text{ICC}_{\text{IAR}} = 0.94$ 95 % CI (0.89 - 0.96)	$\text{SEM}_{\text{IAR}} = 3.0^\circ$ $\text{MDC}_{\text{IAR}} = 8.0^\circ$
D'Oswaldo et al. 1997 ⁵⁶	Arcometer	Persons with orthopedic conditions $n = 16$ intrarater reliability Mean age 13 years BMI = NR Sex (M/F) 8/8 $n = 97$ interrater reliability Mean age/SD 14 years Sex (M/F) 22/27 BMI = NR	$\text{ICC}_{\text{IAR}} = \text{NR}$ $\text{ICC}_{\text{IER}} = \text{NR}$ $r_{\text{INTRA}} = 0.99$ $r_{\text{INTER}} = 0.99$	SEM = NR MDC = NR
Dunk et al. 2004 ³⁶	Photogrammetry GOBER, University of Guelph, Guelph, ON	Patients with kyphosis and scoliosis and for postural rehabilitation $n = 14$ Sex (M/F) 7/7 Female: Mean age $\pm$ SD 22.0 ± 0.8 years; BM (kg) 66.2 ± 12.0 ; Height (cm) 162.0 ± 9.9 ; BMI _C (kg/m^2) 25 Male: Mean age $\pm$ SD 21.6 ± 1.3 years; BM (kg) 76.4 ± 5.2 ; Height (cm) 181.3 ± 4.4 BMI _C (kg/m^2) 23	$\text{ICC}_{\text{IAR}} = 0.51$ female $\text{ICC}_{\text{IAR}} = 0.35$ male	SEM = NR MDC = NR
Dunk et al. 2005 ⁷⁷	Photogrammetry GOBER, University of Waterloo, Waterloo, Ontario.	Healthy and active young adults $n = 20$ Mean age/SD Sex (M/F) 10/10 Female: Mean age $\pm$ SD 21.8 ± 0.6 years; BM(kg) 57.5 ± 8.5 ; Height (cm) 163.6 ± 6.8 ; BMI _C (kg/m^2) 21 Male: Mean age $\pm$ SD 22.6 ± 1.3 years; BM (kg) 76.7 ± 5.1 ; Height (cm) 179.1 ± 3.3 ; BMI _C (kg/m^2) 23	$\text{ICC}_{\text{IAR}} = 0.63$ female $\text{ICC}_{\text{IAR}} = 0.72$ male	SEM = NR MDC = NR
Elpeze, G et al. 2023 ⁷⁸	Flexicurve Angle (FA) Smartphone (SP-app) protractor software of smartphone inclinometer	Healthy and active young adults $n = 60$ Mean age $\pm$ SD 21.92 ± 1.50 BMI (kg/m^2) 22.74 ± 3.46 Sex (M/F) 35/25 Subjects with thoracic kyphosis $\geq 30^\circ$	$\text{ICC}_{\text{IARFA}} = 0.96$ 95 % CI (0.90 – 0.96) $\text{ICC}_{\text{IERFA}} = 0.91$ 95 % CI (0.85 – 0.94) $\text{ICC}_{\text{IARSP}} = 0.96$ 95 % CI (0.93 – 0.97) $\text{ICC}_{\text{IERSP}} = 0.96$ 95 % CI (0.94 – 0.97)	SEM = NR MDC = NR SEM = NR MDC = NR
Faramarzi et al. 2020 ⁵⁷	Smartphone Goniometer-Pro app	$n = 20$ intrarater reliability $n = 20$ interrater reliability Mean age $\pm$ SD 25.1 ± 2.1 years; BMI (kg/m^2) 22.5 ± 2 . Sex (M/F) NR	$\text{ICC}_{\text{IAR}} = 0.88$ 95 % CI (0.75 – 0.95) $\text{ICC}_{\text{IER}} = 0.91$ 95 % CI (0.82 – 0.96)	SEM = NR MDC = NR
Gravina et al. 2017 ⁷⁹	Analog Inclinator	Persons with prescription for an X-ray $n = 139$ Mean age $\pm$ SD 12.5 ± 2.5 years BMI = NR Sex (M/F) 40/99 Normal subjects and with spinal deformities ($n = 41$ - no spine pathology; $n = 11$ - Scheuermann's disease; $n = 38$ - postural hyperkyphosis; $n = 49$ - mild idiopathic scoliosis)	$\text{ICC}_{\text{IAR}} = \text{NR}$ $\text{ICC}_{\text{IER}} = \text{NR}$ $r_{\text{INTRA}} = 0.83$ $r_{\text{INTER}} = 0.84$	SEM = NR MDC = NR
Greendale et al. 2011 ¹²	Debrunner Kyphometer (DK) Flexicurve index (FI) Flexicurve angle (FA)	$n = 113$ intrarater reliability Mean age/SD 75.3 ± 7.5 years BMI (kg/m^2) 26.5 ± 4.5 Sex (M/F) 22/92 $n = 54$ interrater reliability Mean age/SD 75.5 ± 7.7 years BMI (kg/m^2) 26.1 ± 4.3	$\text{ICC}_{\text{IARDK}} = 0.98$ $\text{ICC}_{\text{IARFI}} = 0.96$ $\text{ICC}_{\text{IARFA}} = 0.96$ $\text{ICC}_{\text{IERDK}} = 0.98$ $\text{ICC}_{\text{IERFI}} = 0.96$ $\text{ICC}_{\text{IERFA}} = 0.96$	SEM = NR MDC = NR

(continued on next page)

Table 2 (continued)

Authors and year of the study	Instrument	Study Population	Intrarater and Interrater Reliability	SEM/MDC
Hannink et al. 2019 ³⁰	Microsoft Kinect Sensor index	Sex (M/F) 9/45 Persons with kyphosis > 40° <i>n</i> = 37 Mean age/SD 51.7 ± 20.6 years BMI (kg/m ²) 24.9 ± 3.3 Sex (M/F) 57 % were female	ICC _{IAR} = 0.96 95 % CI (0.92 – 0.97) ICC _{IER} = 0.97 95 % CI (0.95 – 0.98)	SEM = NR MDC _{IAR} = 1.49° SEM = NR MDC _{IER} = 1.50°
Heitz et al. 2018 ³⁷	Photogrammetry Software Clinical Photographic Postural Assessment Tool	Participants without neurological conditions <i>n</i> = 41 (<i>n</i> = 35 - right side) Mean age/SD 13 ± 2 years BM (kg) 43 ± 10 Height (cm) 152 ± 11 BMI _C (kg/m ²) 18 Sex (M/F) 3/38	ICC _{IAR} = 0.85	SEM = 2.4° MDC _(CI90 %) = 5.6°
Hinman et al. 2004 ³⁵	Flexicurve Index	<i>n</i> = 51 (25 pre-menopausal/ 26 post-menopausal) Pre-menopausal Mean age/SD 29.2 years BMI = NR Sex (M/F) 0/25 Healthy women Post-menopausal Mean age/SD 72.3 years BMI = NR Sex (M/F) 0/26	ICC _{IER} = 0.94 95 % CI (0.90 – 0.96)	SEM = NR MDC = NR
Iunes et al. 2005 ³⁵	Photogrammetry ALCimagem-2000 Manipulando Imagens, versão 1,5	<i>n</i> = 21 Mean age/SD 24.19 ± 1.3 years BM (kg) 59.10 ± 12.27 Height (m) 1.66 ± 0.05 BMI _C (kg/m ²) 21 Healthy adults Sex (M/F) 4/17	ICC _{IAR} = 0.32 ICC _{IER} = 0.60	SEM = NR MDC = NR
Kellis et al. 2008 ³⁰	Spinal Mouse	<i>n</i> = 81 Mean age/SD 10.62 ± 1.73 years BM (kg) 41.8 ± 9.3; Height (m) 1.47 ± 0.12 BMI _C (kg/m ²) 19 Sex (M/F) 81/0 Healthy boys	ICC _{IAR} = 0.87 ICC _{IER} = 0.89	SEM _{IAR} = 2.79° MDC = NR SEM _{IER} = 1.47° MDC = NR
Korovessis et al. 2001 ²⁰	Debrunner Kyphometer	<i>n</i> = 90 (<i>n</i> = 35 intrarater reliability. <i>n</i> = 90 interrater reliability) Mean age/SD 15 ± 2.6 years BMI = NR Sex (M/F) 44/46 Adolescents with round back or poor sagittal back appearance	ICC _{IAR} = 0.92 ICC _{IER} = 0.84	SEM = NR MDC = NR
Lewis et al. 2010 ²⁶	Analog Inclinator	<i>n</i> = 90 (<i>n</i> = 45 Adults with shoulder pain) Mean age/SD 43 (19 - 84) years; BM (kg) 71.4; Height (m) 1.7 (range 1.5 - 1.9) BMI _C (kg/m ²) 24 Sex (M/F) 22/23 <i>n</i> = 90 (<i>n</i> = 45 Adults without shoulder pain) Mean age/SD 32 (range 23–56) years; BM (kg) 70.4 Height (m) 1.7 BMI _C (kg/m ²) 24 Sex (M/F) 21/24	ICC _{IAR} = 0.97 95 % CI (0.94 – 0.98) ICC _{IAR} = 0.97 95 % CI (0.95 – 0.99)	SEM = 1.7° MDC = NR SEM = 1.0° MDC = NR
Lewis et al. 2005 ²⁵	Analog Inclinator	<i>n</i> = 120 (<i>n</i> = 15 Adults with shoulder pain) Mean age/SD 48.9 ± 15.2 years; BM (kg) 74.5 ± 12.7 Height(m) 171.2 ± 9.7; BMI _C (kg/m ²) 25 Sex (M/F) 35/25 (<i>n</i> = 15 Adults without shoulder pain) Mean age/SD 34.1 ± 9.9 years BM (kg) 67.8 ± 13.4; Height (m) 170.9 ± 10.4 BMI _C (kg/m ²) 23 Sex (M/F) 29/31	Subjects with symptoms ICC _{IAR} = 0.94 95 % CI (0.83 – 0.98) Subjects without symptoms ICC _{IAR} = 0.96 95 % CI (0.91 – 0.98)	SEM with symptoms 2.5° MDC = NR SEM without symptoms 1.5° MDC = NR
Lundon et al. 1998 ²¹	Debrunner Kyphometer (DK) Flexicurve angle (FA)	<i>n</i> = 26 Mean age/SD 18 - 56 years BMI = NR Sex (M/F) 0/26 Postmenopausal women with diagnosis of osteoporosis	ICC _{IARDK} = 0.99 ICC _{IARFA} = 0.96 ICC _{IERDK} = 0.88 ICC _{IERFA} = 0.87	SEM = NR MDC = NR
MacIntyre et al. 2014 ⁸¹	Digital inclinometer	<i>n</i> = 36 Mean age/SD 69 ± 8.1 years BMI = NR Sex (M/F) 86 % were women Adults at risk for osteoporotic fracture (89 % osteoporotic/ 11 % osteopenic)	ICC _{IAR} = 0.91 95 % CI (0.84 - 0.95)	SEM _{IAR} = 3.5° (2.90 - 4.6°) MDC _(CI90 %) = 8.2°

(continued on next page)

Table 2 (continued)

Authors and year of the study	Instrument	Study Population	Intrarater and Interrater Reliability	SEM/MDC
Mannion et al. 2004 ³²	Spinal Mouse	$n = 20$ Mean age/SD Males 45.4 ± 7.7 years BMI (kg/m^2) 26.5 ± 5.2 Females 38.2 ± 7.6 years BMI (kg/m^2) 22.9 ± 5.7 Sex (M/F) 9/11 Healthy volunteers	$\text{ICC}_{\text{IAR}} = 0.88$ 95 % CI (0.67 - 0.94) $\text{ICC}_{\text{IER}} = 0.87$ 95 % CI (0.70 - 0.95)	$\text{SEM}_{\text{IAR}} = 2.8^\circ$ (2.1 - 4.0) MDC = NR $\text{SEM}_{\text{IER}} = 2.7^\circ$ (2.0 - 3.9) MDC = NR
Mellin G, 1986 ²⁷	Analog Inclinator	$n = 25$ ($n = 10$ intratester reliability; $n = 15$ interrater reliability) Mean age/SD 31.3 ± 5.8 years BM (kg) 67.8 ± 15.4 Height (cm) 169.1 ± 9.1 BMI_C (kg/m^2) 23 Healthy adults Sex (M/F) 9/16	$r_{\text{INTRA}} = 0.92$ $r_{\text{INTER}} = 0.83$	SEM = NR MDC = NR
Nair et al. 2017 ⁹⁶	Analog Inclinator	$n = 28$ Mean age/SD 69.7 ± 10.6 years BMI (kg/m^2) 26.3 ± 6.2 Sex (M/F) 16/12 Subjects with Parkinson Disease	$\text{ICC}_{\text{IER}} = 0.779$ 95 % CI (0.57 - 0.89)	SEM = NR MDC = 13.9°
Ohlén et al. 1989 ²²	Debrunner Kyphometer	$n = 31$ Mean age/SD 32 ± 11 years BMI = NR Sex (M/F) 10/21 Healthy adults	ICC = NR $r_{\text{IAR}} = 0.92$ $r_{\text{IER}} = 0.94$	SEM = NR MDC = NR
Perriman et al. 2010 ³¹	Electrogoniometer	$n = 12$ Mean age/SD 40.7 (25–61) years; BM (kg) 70.9 (50–95) Height (cm) 170.0 (156–186); BMI_C (kg/m^2) 24.5 Sex (M/F) 4/8 Healthy adults	$\text{ICC}_{\text{IAR}} = 0.90$ 95 % CI (0.70 - 0.97)	SEM = NR MDC = NR
Pakelöglu et al. 2023 ⁸³	Flexicurve Angle (FA) Smartphone-app (SP) Goniometer Pro app	$n = 30$ Mean age/SD 21.13 ± 1.78 years BMI (kg/m^2) 21.97 ± 3.17 Height (cm) 173.23 ± 9.54 Sex (M/F) 13/17 Healthy and asymptomatic participants	$\text{ICC}_{\text{IARFA}} = 0.87$ 95 % CI (0.75 - 0.93) $\text{ICC}_{\text{IERFA}} = 0.62$ 95 % CI (0.20 - 0.82) $\text{ICC}_{\text{IARSP}} = 0.90$ 95 % CI (0.80 - 0.95) $\text{ICC}_{\text{IERSP}} = 0.87$ 95 % CI (0.73 - 0.94) $\text{ICC}_{\text{IER}} = 0.94$	$\text{SEM}_{\text{IARFA}} = 1.73^\circ$ $\text{MDC}_{\text{IARFA}} = 3.39^\circ$ $\text{SEM}_{\text{IERFA}} = 1.59^\circ$ $\text{MDC}_{\text{IERFA}} = 3.11^\circ$ $\text{SEM}_{\text{IARSP}} = 1.48^\circ$ $\text{MDC}_{\text{IARSP}} = 2.90^\circ$ $\text{SEM}_{\text{IERSP}} = 1.60^\circ$ $\text{MDC}_{\text{IERSP}} = 3.13^\circ$ SEM = 1.66cm MDC _{IER} = 4.60cm
Prowse et al. 2018 ³³	Baseline® Body Level/Scoliosis meter	$n = 31$ Mean age/SD 13.6 ± 0.6 years BMI = NR Sex (M/F) 4/27 Adolescent with scoliosis	$\text{ICC}_{\text{IAR}} = 0.90$ 95 % CI (0.87 - 0.97)	SEM = NR MDC = NR
Purser et al. 1999 ³⁴	Debrunner Kyphometer	$n = 24$ Mean age/SD 68 ± 4 years BMI = NR Sex (M/F) 3/21 Community-dwelling elderly $n = 15$ Mean age/SD 75 ± 6 years BMI = NR Sex (M/F) 13/2 Community-dwelling with Parkinson disease $n = 12$ Mean age/SD 82 ± 4 years BMI = NR Sex (M/F) 0/12 Subjects with vertebral osteoporosis $n = 14$ Mean age/SD 74 ± 6 years BMI = NR Sex (M/F) 12/2 Nursing home residents	Community-dwelling elderly persons $\text{ICC}_{\text{IAR}} = 0.96$ Community-dwelling with Parkinson disease $\text{ICC}_{\text{IAR}} = 0.95$ Subjects with vertebral osteoporosis $\text{ICC}_{\text{IAR}} = 0.92$ Nursing home residents $\text{ICC}_{\text{IAR}} = 0.91$ Overall ICC = 0.95	SEM = NR MDC = NR
Quek et al. 2017 ³⁸	Flexicurve Angle (FA) Flexicurve Index (FI) Microsoft Kinect Sensor Angle (MKA) Microsoft Kinect Sensor Index (MKI)	$n = 33$ ($n = 29$ intratester reliability) Mean age/SD 31 ± 11.0 years BM (kg) 64.2 ± 12.0 Height (cm) 170.2 ± 8.2 BMI_C (kg/m^2) 22	$\text{ICC}_{\text{IARFA}} = 0.83$ 95 % CI (0.63 - 0.92) $\text{ICC}_{\text{IARFI}} = 0.83$ 95 % CI (0.63 - 0.92) $\text{ICC}_{\text{IARMKA}} = 0.96$ 95 % CI (0.92 - 0.98)	$\text{SEM}_{\text{FA}} = 0.99^\circ$ $\text{MDC}_{\text{FA}} = 2.7^\circ$ $\text{SEM}_{\text{FI}} = 1.11^\circ$ $\text{MDC}_{\text{FI}} = 3.1^\circ$ $\text{SEM}_{\text{MKA}} = 0.69^\circ$ $\text{MDC}_{\text{MKA}} = 1.9^\circ$

(continued on next page)

Table 2 (continued)

[illegible]

(continued on next page)

Table 2 (continued)

Authors and year of the study	Instrument	Study Population	Intrarater and Interrater Reliability	SEM/MDC
Tabard-Fougere et al. 2011, ⁹⁷	Analog Inclinator	Mean age/SD 8.2 ± 1.0 years BMI = NR Sex (M/F) 47/44 Healthy volunteers n = 51	ICC _{IER} = 0.92 95 % CI (0.86 – 0.96)	SEM _{IER} = 0.9° MDC = NR
		Mean age/SD 13.5 (2.0) years BMI (kg/m ²) 18.9 ± 2.8 Sex (M/F) 19/32 Adolescent with idiopathic scoliosis n = 32	ICC _{IAR} = 0.98 95 % CI (0.97 - 0.98)	SEM = NR MDC = NR
Takatalo et al. 2020 ⁹¹	Digital inclinometer	Mean age/SD 39 ± 9.2 years; BMI (kg/m ²) 24.5 ± 3.2 Sex (M/F) 16/16 Persons with pain in thoracic spine n = 56	ICC _{IAR} = 0.83 95 % CI (0.66 - 0.92) ICC _{IER} = 0.82 95 % CI (0.64 - 0.91)	SEM _{IAR} = 3.09° MDC = NR SEM _{IER} = 3.18° MDC = NR
Teixeira et al. 2007 ⁹⁸	Flexicurve Angle	Mean age/SD 66.7 ± 9.37 years BMI = NR Sex (M/F) 21/35 Healthy elderly n = 30	ICC _{IAR} = 0.87 ICC _{IER} = 0.94	SEM = NR MDC = NR
Temporiti et al. 2023 ⁹²	Photogrammetry BHOHB system (Bhohb S.r.l., Italy)	Mean age/SD 22.3 years ± 9.0 years; Mean weight 64.9 kg, SD: 9.04 kg Mean height 173.2 cm, SD: 8.1 cm BMI _C (kg/m ²) 21.7 Sex (M/F) 15/15 Healthy adult volunteers n = 102 (n = 10 intrarater reliability; n = 10 interrater reliability)	ICC _{IAR} = 0.98 95 % CI (0.96 – 0.99)	SEM = 0.78° MDC = NR
Todd et al. 2015 ⁶⁹	Debrunner Kyphometer	Mean age ± SD (reliability) 18.3 ± 1.13 years BMI (kg/m ²) 22.9 ± 3.12 Sex (M/F) NR for reliability Young athletic elite alpine skiers n = 71 (DB); n = 72 (FI); Mean age/SD 77.8 ± 7.1 years BMI (kg/m ²) 25.3 ± 4.6 Sex (M/F) 20/52 Persons recruited from community with thoracic kyphosis n = 17	ICC _{IAR} = 0.83 95 % CI (0.30 – 0.96) ICC _{IER} = 0.96 95 % CI (0.85 – 0.99)	SEM = NR MDC = NR
Tran et al. 2016 ⁷⁰	Debrunner Kyphometer (DK) Flexicurve Index (FI)	Mean age/SD 77.8 ± 7.1 years BMI (kg/m ²) 25.3 ± 4.6 Sex (M/F) 20/52 Persons recruited from community with thoracic kyphosis n = 17	ICC _{IERFI} = 0.93 ICC _{IERDB} = 0.99	SEM = NR MDC = NR
van Baalen et al. 2023 ⁹³	Analog Inclinator AI) Smartphone (SM-app)	Mean age/SD 23.7 ± 2.3 years; BMI (kg/m ²) = 22.3 ± 1.6; Height 1.69 (m) ± 0.1 Sex (M/F) 13/4 Asymptomatic volunteers n = 40 (n = 20 intrarater reliability) Mean age/SD 23.2 ± 3.4 years BMI (kg/m ²) 24.9 ± 3.6 (male) BMI (kg/m ²) 22.5 ± 4.5 (female) Sex (M/F) 14/26 Healthy students n = 1101 (n = 10 intrarater reliability) Mean age/SD ages of 8–16 BMI NR Sex (M/F) 565/536 Healthy children n = 71 Mean age/SD NR Sex (M/F) NR Teenagers with or without visible spinal disorder n = 26 Mean age/SD 67.1 years BM (kg) 59.9 ± 10.6 Height (cm) 158.6 ± 7.7 BMI _C (kg/m ²) 23 Sex (M/F) 0/26 Women who were enrolled in the Trym Gym Osteoporosis Exercise Program	ICC _{IARAI} = 0.92 95 % CI (0.84 – 0.97) ICC _{IERAI} = 0.81 95 % CI (0.55 – 0.93) ICC _{IARSP} = 0.94 95 % CI (0.87 – 0.97) ICC _{IERSP} = 0.67 95 % CI (0.08 – 0.89) ICC _{IAR} = 0.96 95 % CI (0.92 – 0.98)	SEM _{IARAI} = 1.7° MDC _{IARAI} = 4.7° SEM _{IERAI} = 2.6° MDC _{IERAI} = 7.1° SEM _{IARSP} = 1.5° MDC _{IARSP} = 4.3° SEM _{IERSP} = 3.2° MDC _{IERSP} = 9.0° SEM = 1.7° MDC = NR
van Blommestein et al. 2012 ⁹⁴	Analog Inclinator	Mean age/SD 33 ± 11.23 years; BM (kg) 72 ± 12; Height 172 (cm) ± 11 BMI _C (kg/m ²) 24 Sex (M/F) 15/15 Asymptomatic volunteers n = 40 (n = 20 intrarater reliability) Mean age/SD 23.2 ± 3.4 years BMI (kg/m ²) 24.9 ± 3.6 (male) BMI (kg/m ²) 22.5 ± 4.5 (female) Sex (M/F) 14/26 Healthy students n = 1101 (n = 10 intrarater reliability) Mean age/SD ages of 8–16 BMI NR Sex (M/F) 565/536 Healthy children n = 71 Mean age/SD NR Sex (M/F) NR Teenagers with or without visible spinal disorder n = 26 Mean age/SD 67.1 years BM (kg) 59.9 ± 10.6 Height (cm) 158.6 ± 7.7 BMI _C (kg/m ²) 23 Sex (M/F) 0/26 Women who were enrolled in the Trym Gym Osteoporosis Exercise Program	ICC _{IARDI} = 0.8 ICC _{IARSP} = 0.8	SEM = NR MDC = NR
Was et al. 2016 ³⁹	Digital Inclinator (DI) Smartphone (SP-app) Android 4.0.3 software with a built-in accelerometer	Mean age/SD 23.2 ± 3.4 years BMI (kg/m ²) 24.9 ± 3.6 (male) BMI (kg/m ²) 22.5 ± 4.5 (female) Sex (M/F) 14/26 Healthy students n = 1101 (n = 10 intrarater reliability) Mean age/SD ages of 8–16 BMI NR Sex (M/F) 565/536 Healthy children n = 71 Mean age/SD NR Sex (M/F) NR Teenagers with or without visible spinal disorder n = 26 Mean age/SD 67.1 years BM (kg) 59.9 ± 10.6 Height (cm) 158.6 ± 7.7 BMI _C (kg/m ²) 23 Sex (M/F) 0/26 Women who were enrolled in the Trym Gym Osteoporosis Exercise Program	ICC _{IARDI} = 0.8 ICC _{IARSP} = 0.8	SEM = NR MDC = NR
Willner and Johnson, 1983 ¹⁸	Spinal Pantograph	Mean age/SD 67.1 years BM (kg) 59.9 ± 10.6 Height (cm) 158.6 ± 7.7 BMI _C (kg/m ²) 23 Sex (M/F) 0/26 Women who were enrolled in the Trym Gym Osteoporosis Exercise Program	ICC _{IAR} = NR ICC _{IER} = NR	SEM = NR MDC = NR
Willner Stig, 1981 ¹⁷	Spinal Pantograph	Mean age/SD 67.1 years BM (kg) 59.9 ± 10.6 Height (cm) 158.6 ± 7.7 BMI _C (kg/m ²) 23 Sex (M/F) 0/26 Women who were enrolled in the Trym Gym Osteoporosis Exercise Program	ICC _{IAR} = NR ICC _{IER} = NR	SEM = NR MDC = NR
Yanagawa et al. 2000 ⁴²	Flexicurve index	Mean age/SD 67.1 years BM (kg) 59.9 ± 10.6 Height (cm) 158.6 ± 7.7 BMI _C (kg/m ²) 23 Sex (M/F) 0/26 Women who were enrolled in the Trym Gym Osteoporosis Exercise Program	ICC _{IAR} = 0.93 95 % CI (0.85 – 0.97)	SEM = NR MDC = NR

Note. NR, Not reported; BM, Body mass; BMI, Body mass index; BMI_C, Body mass index calculated; 95 % CI, 95 % confidence intervals; ICC, Intraclass correlation coefficient; ICC_{IAR}, Intrarater ICC; ICC_{IER}, Interrater ICC; ICC_{IARFA}, Intrarater ICC flexicurve angle; ICC_{IERFA}, Interrater ICC flexicurve angle; ICC_{IARFI}, Intrarater ICC flexicurve index; ICC_{IERFI}, Interrater ICC flexicurve index; ICC_{IARDID}, Intrarater ICC dual digital inclinometer; ICC_{IERDDI}, Interrater ICC dual digital inclinometer; ICC_{IARI}, Intrarater ICC analog inclinometer; ICC_{IERAI}, Interrater ICC analog inclinometer; ICC_{IARSP}, Intrarater ICC smartphone-app; ICC_{IERSP}, Interrater ICC smartphone-app; ICC_{IARDK}, Intrarater ICC debrunner kyphometer; ICC_{IERDK}, Interrater ICC debrunner kyphometer; ICC_{IARMKSA}, Intrarater ICC microsoft kinect sensor angle; ICC_{IERMKS}, Interrater ICC microsoft kinect sensor index; ICC_{IARDI}, Intrarater ICC digital inclinometer; CI, Confidence interval 95 %; SEM, Standard error of measurement; SEM_{IAR}, Standard error of measurement of intrarater ICC; SEM_{IER}, Standard error of measurement of interrater ICC; SEM_{IARFA}, SEM_{IAR} flexicurve angle; SEM_{IERFA}, SEM_{IER} flexicurve angle; SEM_{IARFI}, SEM_{IAR} flexicurve index; SEM_{IERFI}, SEM_{IER} flexicurve index; SEM_{IARMKA}, SEM_{IAR} microsoft kinect sensor angle; SEM_{IERMKI}, SEM_{IER} microsoft kinect sensor index; SEM_{IARSP}, SEM_{IAR} smartphone app; SEM_{IERSP}, SEM_{IER} smartphone-app; MDC, Minimal detectable change; MDC_{IAR}, Intrarater MDC; MDC_{IER}, Interrater MDC; MDC_{IARFA}, MDC_{IAR} flexicurve angle; MDC_{IARFI}, MDC_{IAR} flexicurve index; MDC_{IARMKA}, MDC_{IAR} Microsoft kinect sensor angle; MDC_{IARMKI}, MDC_{IAR} microsoft kinect sensor index; r_{INTRA} , Intrarater Correlation; r_{INTER} , Interrater Correlation.

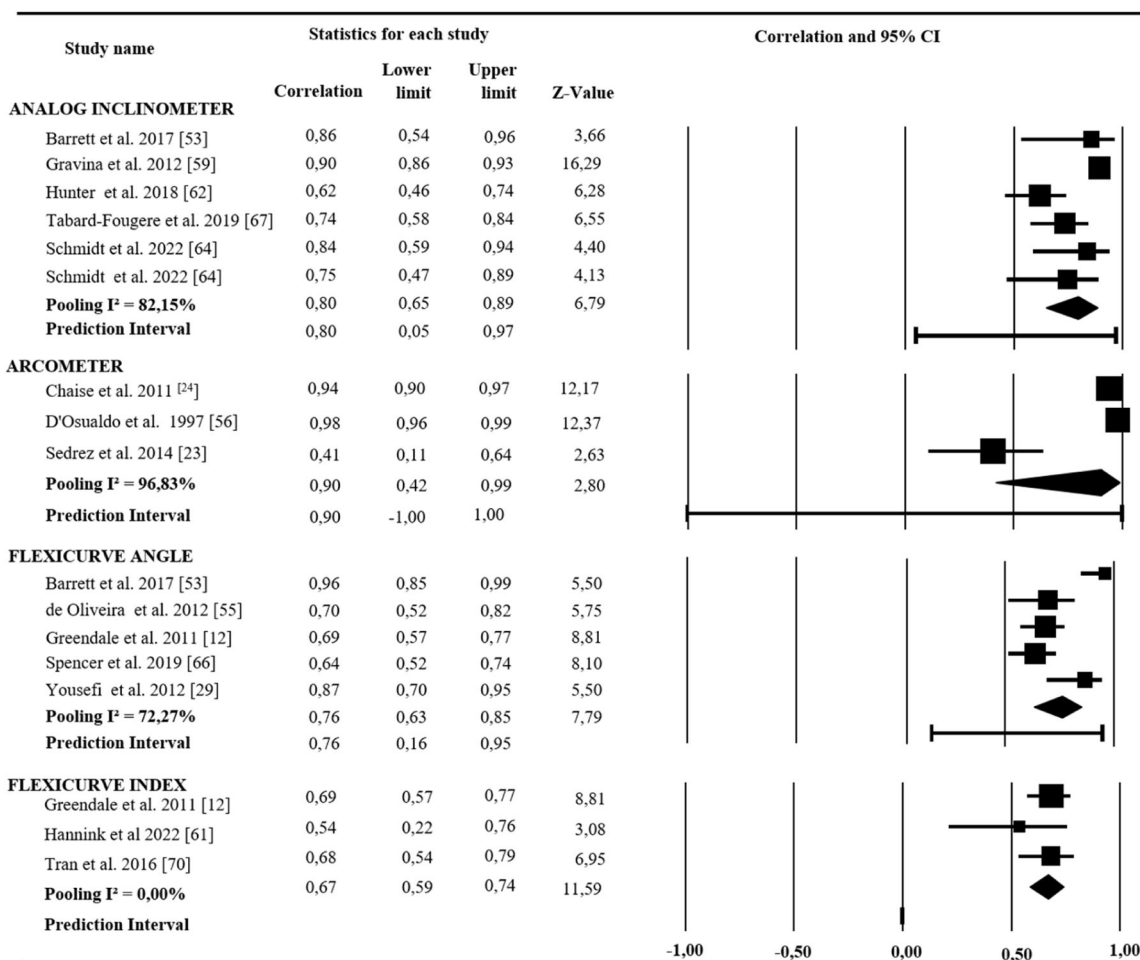


Fig. 2. - Results of the sensitive analysis of the validity for the different types of instruments.

studies. These data were grouped into six meta-analyses, one for each instrument. The following instruments demonstrated excellent inter-rater reliability: Analog Inclinometer, Digital Inclinometer, Flexicurve Angle, Flexicurve Index, Photogrammetry, Smartphone app, and Spinal Mouse (Fig. 4). Moreover, the inter-rater reliability was not assessed in studies that used the Kypholordometer⁵² and Electrogoniometer.³¹ The Baseline® Level/Scoliosis,³³ Dual Digital Inclinometer,⁵¹ Microsoft Kinect Sensor,⁸⁰ and Spinal Wheel³² were investigated in only one study each, showing excellent inter-rater reliability (Table 2). The Spinal Pantograph was explored in only one study,¹⁷ but the ICC was not performed. The Arcometer was evaluated in three studies: one did not report the ICC,⁵⁶ and two demonstrated levels of inter-rater reliability ranging from low to excellent (0.25 to 0.98)^{23–24}; however, they did not report the 95 %CI of the ICC, making the meta-analysis unfeasible. The Debrunner Kyphometer was evaluated in six studies,^{12,20–22,69–70} but

only one reported the 95 % CI of the ICC⁶⁹; the meta-analysis was not performed. One study did not report the ICC,²² and the other five showed excellent inter-rater reliability (Table 2).^{12,20–21,69–70} The MDC and SEM were reported for five and seven instruments, respectively (Table 2).

Utility of the instrument

All instruments' measurement properties were investigated and classified according to clinical utility (Supplementary materials 4 and 5). Only the Analog Inclinometer, Flexicurve Angle, and Smartphone app demonstrated excellent levels for all measurement properties (> 0.80) and reported MDC data. The Microsoft Kinect Sensor did not present excellent validity; thus, this instrument was not considered. The Arcometer, Photogrammetry, and Spinal Mouse demonstrated excellent

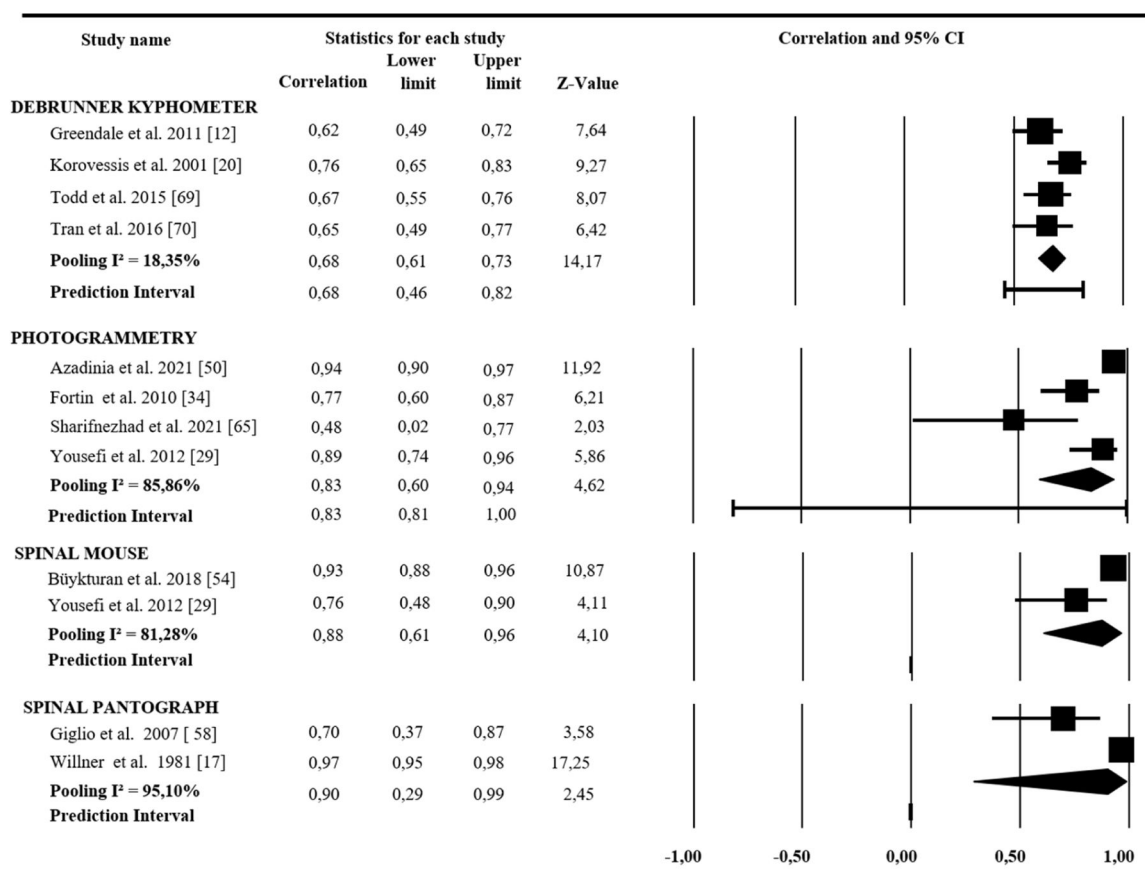


Fig. 2. (continued).

validity and reliability but did not have MDC data reported; therefore, they were not considered. Last, the instruments Baseline® Body Level/ Scoliosis meter, Kypholordometer, Debrunner Kyphometer, Digital Inclinator, Dual Digital Inclinator, Electrogoniometer, Flexicurve Index, Spinal Pantograph, and Spinal Wheel did not present excellent validity and reliability levels or one or more measurement properties and cannot be considered helpful for clinical practice. Therefore, only the Analog Inclinator, Flexicurve Angle, and Smartphone app are recommended for use in clinical settings (scores ≥ 9).

Discussion

The present review with meta-analysis investigated the validity, intra- and inter-rater reliability, and clinical utility of instruments designed to measure thoracic kyphosis. In the 72 included studies, 15 instruments had their measurement properties investigated; the Flexicurve Angle and Analog Inclinator were the most investigated. Data from seven instruments were grouped in a meta-analysis for validity and intra-rater reliability and from six instruments for inter-rater reliability.

Most studies investigating validity demonstrated a moderate to strong correlation with the gold standard measure. Some factors may interfere with the correlation between noninvasive instruments and X-ray examinations. For instance, The Cobb angle quantifies the thoracic kyphosis by locating the positioning of the vertebrae on the X-ray. In contrast, the instrument is positioned on the skin and suffers the interference of soft tissue artifacts, which may generate discrepancies between measures.²⁴ Although all studies included in this review described the procedures for assessing thoracic kyphosis, four studies did not declare which vertebral limits were used to measure thoracic kyphosis by X-ray examination.^{34,56,58–59} In addition, clinical measurements and imaging examinations are generally not standardized. Some studies

measured thoracic kyphosis with the instrument positioned between C7 and T12,⁵³ T2/T3 and T11/T12,^{69–70} and from C7 to the curve inflection point.⁷⁰ Although the measurement recommended by Cobb for X-ray examination is from T4 to T12, some measurements presented variations, such as from T1 to T10⁶² and T1 to T12.²³ Another aspect that may interfere with validity is the time interval between the clinical and the gold standard measurement. Although 10 studies did not report this interval, most performed both measurements on the same day. Finally, a strong correlation with the gold standard does not ensure good agreement and measurement accuracy between the two methods.⁵⁰ A few instruments were analyzed using the Bland-Altman to verify the agreement limits. Therefore, further validity studies must perform the Bland-Altman analysis.

The Analog Inclinator, Digital Inclinator, Flexicurve Angle and Index, Photogrammetry, Microsoft Kinect Sensor, Spinal Mouse, and Smartphone app showed excellent levels of intra-rater reliability. Examiner experience and lack of blinding of the examiner and the time interval between measurements may help to explain these findings. Most of the studies included in the intrarater reliability analysis (65.51 %) declared that the rater was experienced in clinical practice or in using the instrument. Regarding blinding, only 14 studies declared the rater was blind to the measurements. Furthermore, most studies (86.20 %) adopted a time interval of up to seven days, allowing control over changes in posture resulting from flexibility and body mass index.³³

The Analog Inclinator, Digital Inclinator, Flexicurve Angle and Index, Photogrammetry, Smartphone app, and Spinal Mouse demonstrated excellent inter-rater reliability. Although differences between examiners' experience may hinder inter-rater reliability, eight studies included in the meta-analysis (44.44 %) used examiners with different experience levels, which suggests that these instruments are user-friendly.^{65,71,73,78,88,90–91,93} Few studies investigated the SEM and the

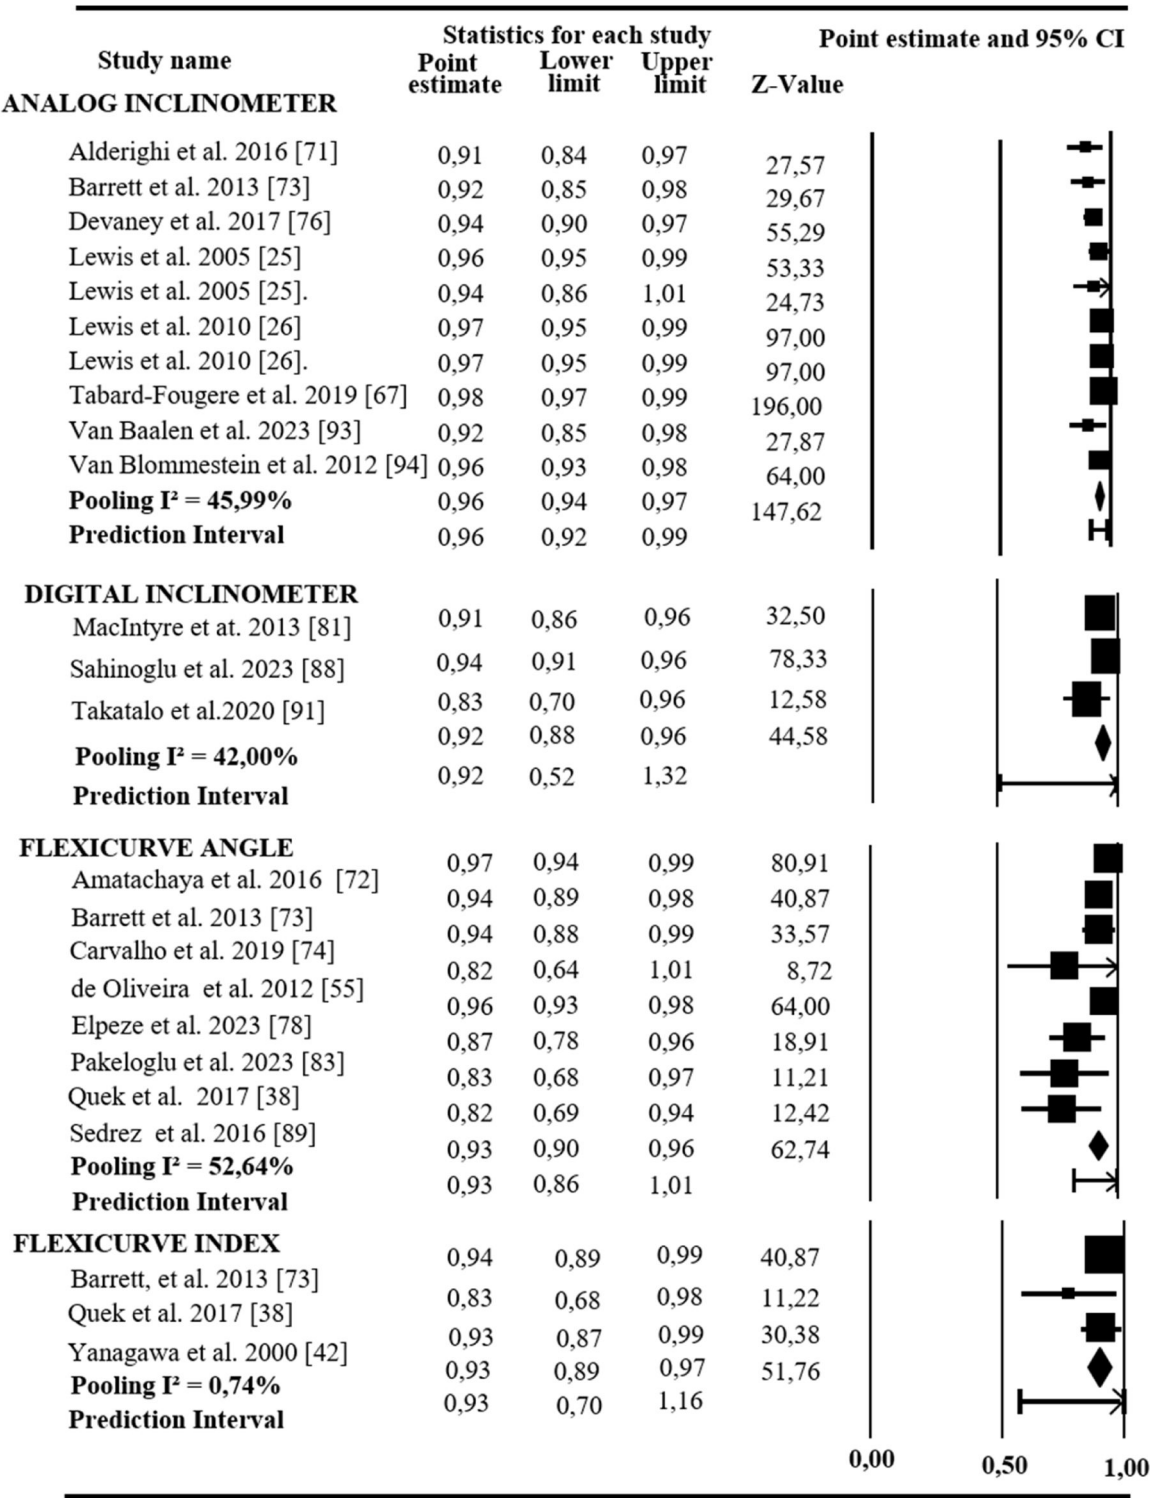


Fig. 3. - Results of the sensitive analysis of intrarater reliability for the different types of instruments.

MDC of the instruments. Some measurement errors may include the experience of the examiner in locating reference points on the skin,⁷¹ the positioning, pressure, and speed in which the instrument is slid over the skin,³² transfer the measurement to the paper (e.g., Flexicurve measurement),⁷³ the location of markers in the software,⁷⁷ and the positioning of the individual.²⁰ Most studies evaluated individuals in a relaxed orthostatic posture. Some studies have observed a positive correlation between thoracic curvatures measured from upright and

relaxed postures and noted that the measurement is significantly smaller when performed from an upright posture.^{76,96} Therefore, the choice of which posture to evaluate should consider that the measurement of the thoracic kyphosis in an upright orthostatic position will reflect structural kyphosis and minimize the effects of muscle weakness.⁷² Regarding clinical utility, this review identified that the Analog Inclinator, Flexicurve Angle, and Smartphone app are suitable for clinical practice. Although the Flexicurve Angle presents MDC and

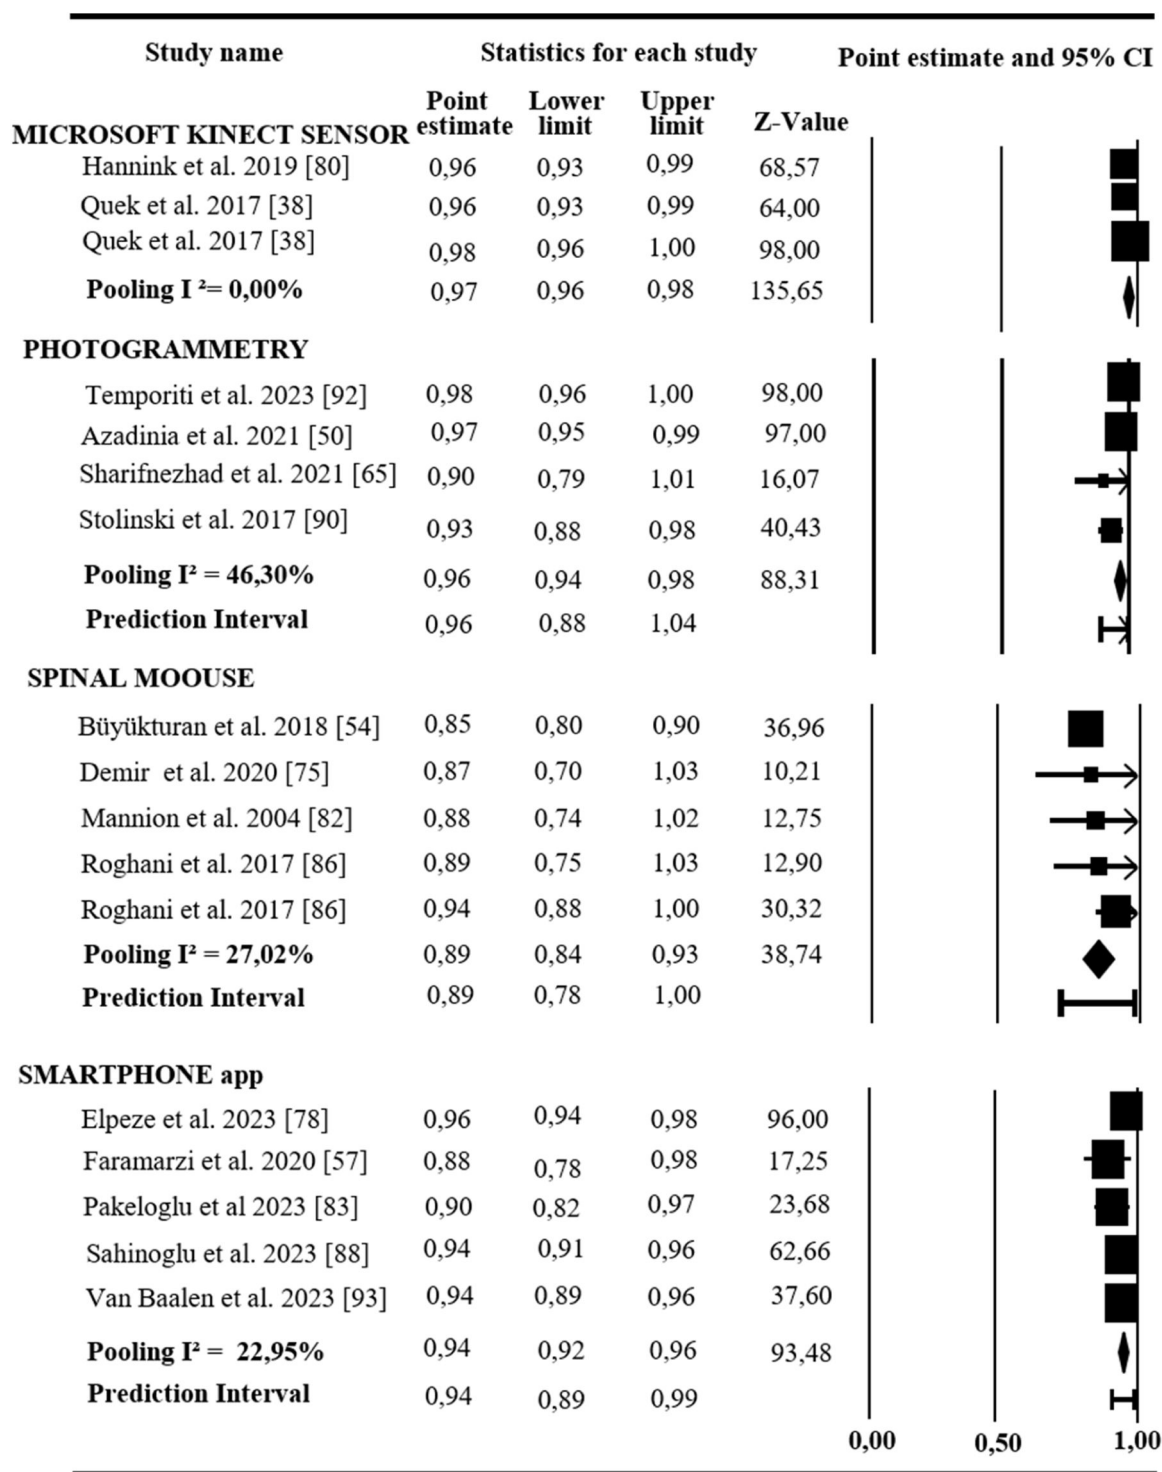


Fig. 3. (continued).

excellent levels of reliability and validity, the agreement between this instrument and the modified Cobb angle by the X-ray using the Bland Altman demonstrated wide limits of agreement.^{53,55,66} Furthermore, the Flexicurve underestimates the magnitude of the thoracic kyphosis angle in the sagittal plane to X-ray, and this may be a problem in clinical settings when precise measurements are required.⁶⁶ Future studies could explore the measurements properties of the Digital Inclinometer and Dual Digital Inclinometer, which have a moderate cost, are portable, easy to administer, do not require specific training, and are often used in clinical settings.

The use of low-cost, portable, and precise clinical instruments can significantly improve patient outcomes by enabling quick, objective assessments and early detection of thoracic kyphosis severity, facilitating timely interventions. Continuous monitoring across various settings, such as clinics or patients' homes, supports frequent adjustments to treatment plans, resulting in better functional and postural outcomes while enhancing treatment adherence. Reliable, standardized measurements reduce intra- and inter-rater variability, ensuring consistent data and evidence-based clinical decisions. Combining precision with efficiency, these tools enable personalized rehabilitation strategies that

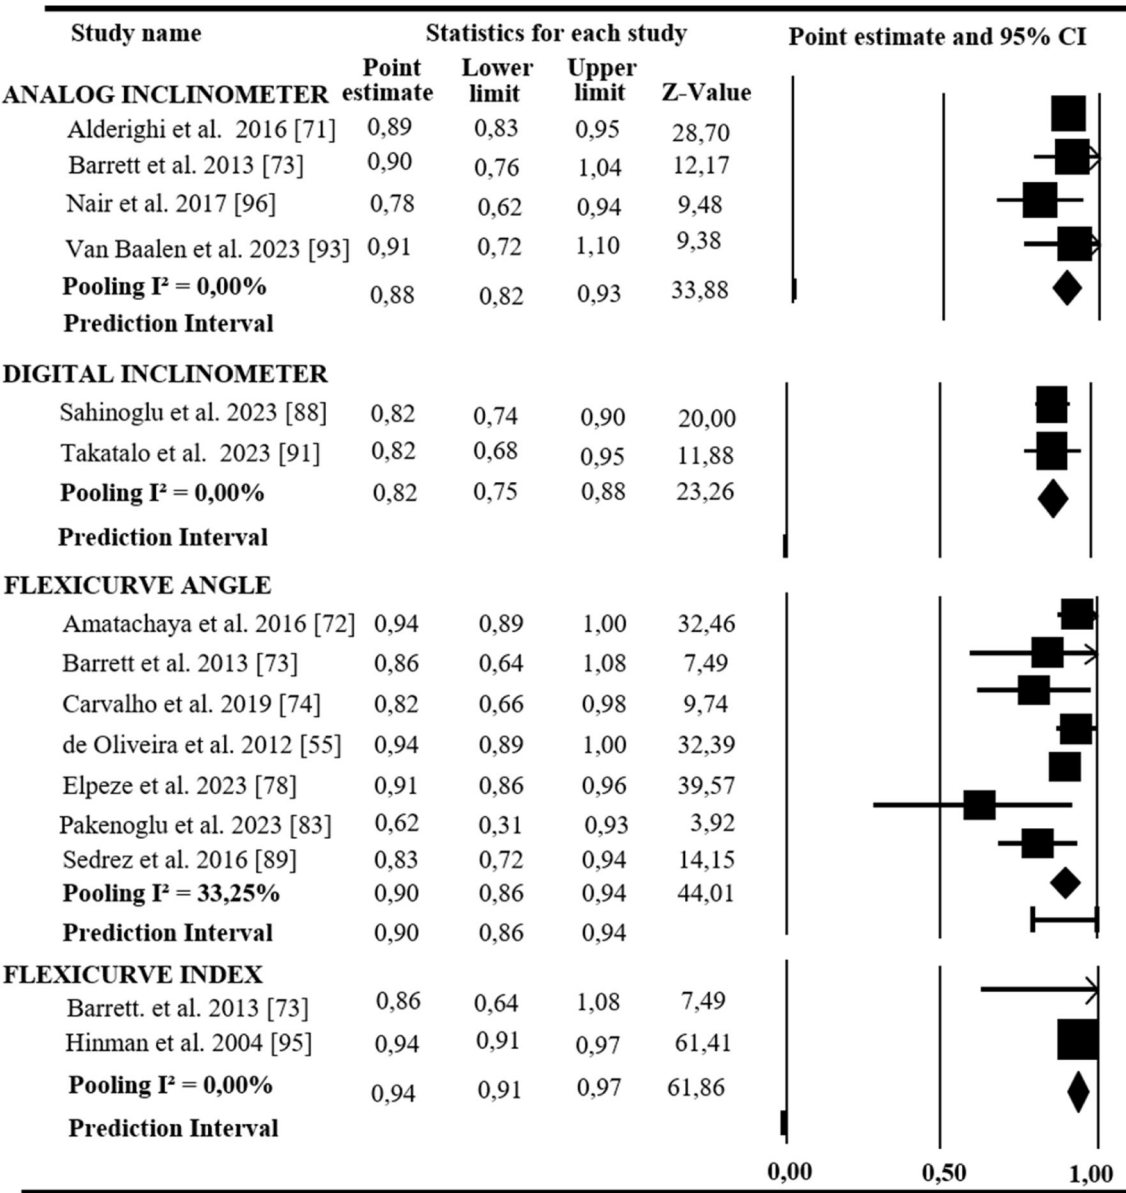


Fig. 4. - Results of the sensitive analysis of the interrater reliability for different types of instruments.

adapt to changes in the patient’s condition.

This review had some limitations. Data extraction was conducted by only one author. In addition, when studies reported the experience of the rater, only the intra-rater reliability from the most experienced was extracted. When not reported, the highest reliability value was extracted, which may have overestimated the intra-rater reliability levels. Furthermore, the meta-analysis did not differentiate between ICC models due to limitations in the available data and the number of included studies, which may have impacted the interpretation of reliability measures. Additionally, subgroup analyses were not conducted due to the limited number of studies and concerns about insufficient statistical power, which could lead to unreliable and non-robust conclusions.⁹⁷

Compared with the Barret et al. review, the present review found a higher number of studies on the topic not only in healthy individuals, but also in patients with disabilities and athletes. However, the

reliability and validity of the instruments are generally specific to the investigated sample. Therefore, generalization of these findings to populations not considered in this review must be conducted cautiously.

Conclusions

The present review demonstrated the validity and intra and inter-rater reliability of 15 clinical instruments for assessing thoracic kyphosis in the sagittal plane. The meta-analysis demonstrated that the Analog Inclinator, Flexicurve Angle and Index, Photogrammetry, and Spinal Mouse are valid and reliable for evaluating thoracic kyphosis in the sagittal plane. The analysis of the instruments’ utility suggests using the Analog Inclinator, Flexicurve Angle, and the Smartphone app to measure thoracic kyphosis in the sagittal plane in clinical settings.

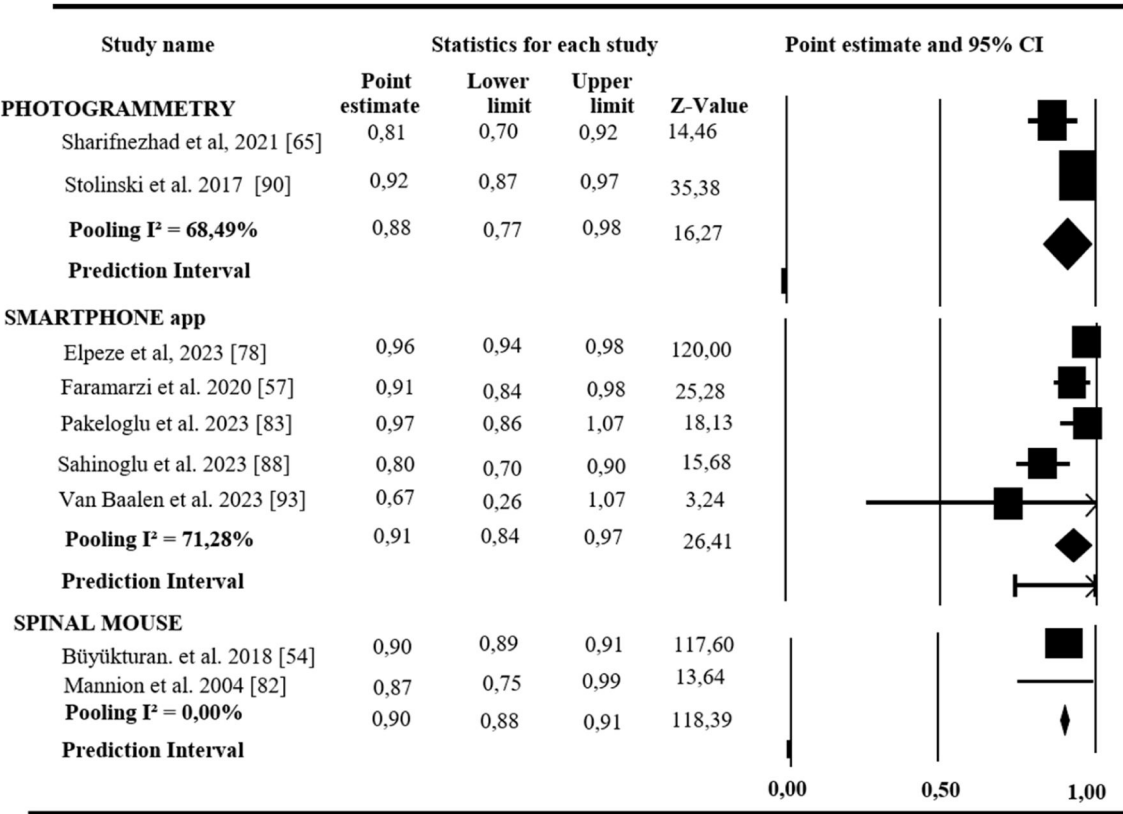


Fig. 4. (continued).

Declaration of competing interest

The authors declare no competing interest.

Supplementary materials

Supplementary material associated with this article can be found, in the online version, at [doi:10.1016/j.bjpt.2025.101246](https://doi.org/10.1016/j.bjpt.2025.101246).

References

1. Perriman DM, Scarvell JM, Hughes AR, Lueck CJ, Dear KBG, Smith PN. Thoracic hyperkyphosis: a survey of Australian physiotherapists. *Physiother. Res Int.* 2012;17:167–178. <https://doi.org/10.1002/pri.529>.

2. Lau KT, Cheung KY, Chan KB, Chan MH, Lo KY, Chiu TTWing. Relationships between sagittal postures of thoracic and cervical spine, presence of neck pain, neck pain severity and disability. *Man Ther.* 2010;15:457–462. <https://doi.org/10.1016/j.math.2010.03.009>.

3. Ryan PJ, Blake G, Herd R, Fogelman I. A clinical profile of back pain and disability in patients with spinal osteoporosis. *Bone.* 1994;15:27–30. [https://doi.org/10.1016/8756-3282\(94\)90887-7](https://doi.org/10.1016/8756-3282(94)90887-7).

4. Balzini L, Vannucchi L, Benvenuti F, Benucci M, Monni M, Cappozzo A, et al. Clinical characteristics of flexed posture in elderly women. *J Am Geriatr Soc.* 2003;51:1419–1426. <https://doi.org/10.1046/j.1532-5415.2003.51460.x>.

5. Culham C, Jimenez G, King H. Thoracic kyphosis, rib mobility, and lung volumes in normal women and women with osteoporosis. *Spine (Phila Pa 1976).* 1994;19:1250–1255.

6. Ryan SD, Fried LP. The impact of kyphosis on daily functioning. *J Am Geriatr Soc.* 1997;45:1479–1486. <https://doi.org/10.1111/j.1532-5415.1997.tb03199.x>.

7. Kado DM, Huang MH, Nguyen Ck, Barrett-Connor E, Greendale GA. Hyperkyphotic posture and risk of injurious falls in older persons: the Rancho Bernardo Study. *J Gerontol - Ser A, Biol Sci Med Sci.* 2007;62:652–657. <https://doi.org/10.1093/gerona/62.6.652>.

8. Kado DM. Hyperkyphosis predicts mortality independent of vertebral osteoporosis in older women. *Ann Intern Med.* 2009;150:681. <https://doi.org/10.7326/0003-4819-150-10-200905190-00005>.

9. González-Gálvez N, Gea-García GM, Marcos-Pardo PJ. Effects of exercise programs on kyphosis and lordosis angle: a systematic review and meta-analysis. *PLoS One.* 2019;14:1–18. <https://doi.org/10.1371/journal.pone.0216180>.

10. Jang HJ, Hughes LC, Oh DW, Kim SY. Effects of corrective exercise for thoracic hyperkyphosis on posture, balance, and well-being in older women: a double-blind, group-Matched design. *J Geriatr Phys Ther.* 2019;42:E17–E27. <https://doi.org/10.1519/JPT.0000000000000146>.

11. Fon GT, Pitt M, Thies A. Thoracic kyphosis: range in normal subjects. *Am Roentgen Ray Soc.* 1980;134:979–983. www.ajronline.org.

12. Greendale GA, Nili NS, Huang MH, Seeger L, Karlamangla AS. The reliability and validity of three non-radiological measures of thoracic kyphosis and their relations to the standing radiological Cobb angle. *Osteoporos Int.* 2011;22:1897–1905. <https://doi.org/10.1007/s00198-010-1422-z>.

13. Roaf R. Vertebral growth and its mechanical control. *J Bone Jt Surg.* 1960;42-B:40–59. <https://doi.org/10.1302/0301-620X.42B1.40>.

14. Koële MC, Lems WF, Willems HC. The Clinical relevance of hyperkyphosis: a narrative review. *Front Endocrinol (Lausanne).* 2020. <https://doi.org/10.3389/fendo.2020.00005>.

15. Winter R, Lovell W, Moe J. Excessive thoracic lordosis and loss of pulmonary function in patients with idiopathic scoliosis. *J Bone Jt Surg 57-A.* 1975:972–977. <https://doi.org/10.2106/0004623-197557070-00016>.

16. Portney LG. *Foundations of Clinical research: Applications to Evidence-Based Practice.* F. A Davis, Philadelphia; 2020. <http://fadvistech.mhmedical.com/content.aspx?aid=1172486561>.

17. Willner S. Spinal pantograph-a non-invasive technique for describing kyphosis and lordosis in the thoraco-lumbar spine. *Acta Orthop.* 1981;52:525–529. <https://doi.org/10.3109/17453678108992142>.

18. Willner S, Johnson B. Thoracic kyphosis and lumbar lordosis during the growth period in children. *Acta Paediatr.* 1983;72:873–878. <https://doi.org/10.1111/j.1651-2227.1983.tb09833.x>.

19. Kado DM, Christianson L, Palermo L, Smith-Bindman R, Cummings SR, Greendale GA. Comparing a supine radiologic versus standing clinical measurement of kyphosis in older women: the fracture intervention trial. *Spine (Phila Pa 1976).* 2006;31:463–467. <https://doi.org/10.1097/01.brs.0000200131.01313.a9>.

20. Korovessis P, Petsinis G, Papazisis Z, Baikousis A. Prediction of thoracic kyphosis using the Debrunner kyphometer. *J Spinal Disord.* 2001;14:67–72. <https://doi.org/10.1097/00002517-200102000-00010>.

21. Lundon KMA, Li AMWY, Bibershtein S. Interrater and intrarater reliability in the measurement of kyphosis in postmenopausal women with osteoporosis. *Spine (Phila Pa 1976).* 1998;23:1978–1985. <https://doi.org/10.1097/00007632-199809150-00013>.

22. Öhlin G, Spangfort E, Tingvall C, Öhlin G, Spangfort E, Tingvall C. Measurement of spinal sagittal configuration and mobility with Debrunner's kyphometer. *Spine (Phila Pa 1976).* 1989;14:580–583.

23. Sedrez JA, Candotti CT, Medeiros FS, Marques MT, Rosa MIZ, Loss JF. Can the adapted arcometer be used to assess the vertebral column in children? *Brazilian J Phys Ther.* 2014;18:538–543. <https://doi.org/10.1590/bjpt-rbf.2014.0060>.

24. Chaise FO, Candotti CT, Torre ML, Furlanetto TS, Pelinson PPT, Loss JF. Validation, repeatability and reproducibility of a noninvasive instrument for measuring thoracic and lumbar curvature of the spine in the sagittal plane. *Brazilian J Phys Ther*. 2011; 15:511–517. <https://doi.org/10.1590/S1413-35552011005000031>.
25. Lewis JS, Green A, Wright C. Subacromial impingement syndrome: the role of posture and muscle imbalance. *J Shoulder Elbow Surg*. 2005;14:385–392. <https://doi.org/10.1016/j.jse.2004.08.007>.
26. Lewis JS, Valentine RE. Clinical measurement of the thoracic kyphosis. A study of the intra-rater reliability in subjects with and without shoulder pain. *BMC Musculoskelet Disord*. 2010;11:1–7. <https://doi.org/10.1186/1471-2474-11-39>.
27. Mellin G. Measurement of thoracolumbar posture and mobility with a Myrin inclinometer. *Spine (Phila Pa 1976)*. 1986;11:759–762.
28. Czaprowski D, Pawlowska P, Gebicka A, Sitarski D, Kotwicki T. Intra- and interobserver repeatability of the assessment of anteroposterior curvatures of the spine using saunders digital inclinometer. *Ortop Traumatol Rehabil*. 2012;14: 145–153. <https://doi.org/10.5604/15093492.992283>.
29. Yousefi MM, Ilbeigi S, Yousefi MM, Mehrshad N, Afzalpour ME, Naghibi SE. Comparing the validity of non-invasive methods in measuring thoracic kyphosis and lumbar lordosis. *Artic. Zahedan J Res Med Sci*. 2012;14:37–42. <https://www.researchgate.net/publication/270875926>.
30. Kellis E, Adamou G, Tziliou G. M. Emmanouilidou, reliability of spinal range of motion in healthy boys using a skin-surface device. *J Manip Physiol Ther*. 2008;31: 570–576. <https://doi.org/10.1016/j.jmpt.2008.09.001>.
31. Perriman DM, Scarvell JM, Hughes AR, Ashman B, Lueck CJ, Smith PN. Validation of the flexible electrogoniometer for measuring thoracic kyphosis. *Spine (Phila Pa 1976)*. 2010;35:633–640. <https://doi.org/10.1097/BRS.0b013e3181d13039>.
32. Sheeran L, Sparkes V, Busse M, Van Deursen R. Preliminary study: reliability of the spinal wheel. A novel device to measure spinal postures applied to sitting and standing. *Eur Spine J*. 2010;19:995–1003. <https://doi.org/10.1007/s00586-009-1241-0>.
33. Prowse A, Aslaksen B, Kierkegaard M, Furness J, Gerdhem P, Abbott A. Reliability and concurrent validity of postural asymmetry measurement in adolescent idiopathic scoliosis. *World J Orthop*. 2017;8:68–76. <https://doi.org/10.5312/wjo.v8.i1.68>.
34. Fortin C, Feldman DE, Cheriet F, Labelle H. Validity of a quantitative clinical measurement tool of trunk posture in idiopathic scoliosis. *Spine (Phila Pa 1976)*. 2010;35:988–994. <https://doi.org/10.1097/BRS.0b013e3181cd2cd2>.
35. Iunes DH, Castro FA, Salgado HS, Moura IC, Oliveira AS, Bevilacqua-Grossi DE. Confiabilidade intra e interexaminadores e retestabilidade da avaliação postural pela fotogrametria. *Rev Bras Fisioter*. 2005;9:327–334.
36. Dunk NM, Chung YY, Compton DS, Callaghan JP. The reliability of quantifying upright standing postures as a baseline diagnostic clinical tool. *J Manip Physiol Ther*. 2004;27:91–96. <https://doi.org/10.1016/j.jmpt.2003.12.003>.
37. Heitz PH, Aubin-Fournier JF, Parent E, Fortin C. Test-retest reliability of posture measurements in adolescents with idiopathic scoliosis. *Spine J*. 2018;18:2247–2258. <https://doi.org/10.1016/j.spinee.2018.05.006>.
38. Quek J, Brauer SG, Treleaven J, Clark RA. The concurrent validity and interrater reliability of the Microsoft Kinect to measure thoracic kyphosis. *Int J Rehabil Res*. 2017;40:279–284. <https://doi.org/10.1097/MRR.0000000000000237>.
39. Waś J, Sitarski D, Ewertowska P, Błoda J, Czaprowski D. Możliwości wykorzystania telefonu komórkowego w badaniu krzywizn strzałkowych kręgosłupa. *Postępy Rehabil*. 2016;30:29–38. <https://doi.org/10.1515/rehab-2015-0053>.
40. Barrett E, McCreesh K, Lewis J. Reliability and validity of non-radiographic methods of thoracic kyphosis measurement: a systematic review. *Man Ther*. 2014;19:10–17. <https://doi.org/10.1016/j.math.2013.09.003>.
41. Moher D, Shamseer L, Clarke M, Ghersi D, Liberati A, Petticrew M, et al. Preferred reporting items for systematic review and meta-analysis protocols (PRISMA-P) 2015 statement. *Syst Rev*. 2015;4:1. <https://doi.org/10.1186/2046-4053-4-1>.
42. Yanagawa TL, Maitland ME, Burgess K, Young L, Hanley D. Assessment of thoracic kyphosis using the flexicurve for individuals with osteoporosis. *Hong Kong Physiother J*. 2000;18:53–57. [https://doi.org/10.1016/S1013-7025\(00\)18004-2](https://doi.org/10.1016/S1013-7025(00)18004-2).
43. Brink Y, Louw QA. Clinical instruments: reliability and validity critical appraisal. *J Eval Clin Pract*. 2012;18:1126–1132. <https://doi.org/10.1111/j.1365-2753.2011.01707.x>.
44. Shiel F, Persson C, Furness J, Simas V, Pope R, Climestein M, et al. Dual energy X-ray absorptiometry positioning protocols in assessing body composition: a systematic review of the literature. *J Sci Med Sport*. 2018;21:1038–1044. <https://doi.org/10.1016/j.jsams.2018.03.005>.
45. Keogh JWL, Cox A, Anderson S, Liew B, Olsen A, Schram B, Furness J. Reliability and validity of clinically accessible smartphone applications to measure joint range of motion: a systematic review. *PLoS One*. 2019;14, e0215806. <https://doi.org/10.1371/journal.pone.0215806>.
46. Higgins JPT. Measuring inconsistency in meta-analyses. *BMJ*. 2003;327:557–560. <https://doi.org/10.1136/bmj.327.7414.557>.
47. Fleiss JL, Levin B, Paik MC. *The measurement of interrater agreement. Statistical Methods Rates Proportions*. Hoboken, New Jersey: John Wiley & Sons; 2004:598–626. <https://doi.org/10.1002/0471445428.ch18>.
48. Tyson S. A systematic review of methods to measure posture. *Phys Ther Rev*. 2003;8: 45–50. <https://doi.org/10.1179/108331903225001390>.
49. Tyson S, Connell L. The psychometric properties and clinical utility of measures of walking and mobility in neurological conditions: a systematic review. *Clin Rehabil*. 2009;23:1018–1033. <https://doi.org/10.1177/0269215509339004>.
50. Azadinia F, Hosseiniabadi M, Ebrahimi I, Mohseni-Bandpei MA, Ghandhari H, Yassin M, et al. Validity and test-retest reliability of photogrammetry in adolescents with hyperkyphosis. *Physiother Theory Pract*. 2021. <https://doi.org/10.1080/09593985.2021.1975337> (Published online).
51. Azadinia F, Kamyab M, Behtash H, Ganjavian MS, Javaheri MRMM, Saleh Ganjavian M, et al. The validity and reliability of noninvasive methods for measuring kyphosis. *J Spinal Disord Tech*. 2014;27:E212–E218. <https://doi.org/10.1097/BSD.0b013e31829a3574>.
52. Barauna M, Sanchez H, Ventura-Silva R, Malusa S. Validade e confiabilidade intra-indivíduo do cifolordometro na avaliacao da convexidade toracica. *Braz J Phys Ther*. 2005;9:319–325.
53. Barrett E, Lenehan B, O'sullivan K, Lewis J, McCreesh K. Validation of the manual inclinometer and flexicurve for the measurement of thoracic kyphosis. *Physiother Theory Pract*. 2018;34:301–308. <https://doi.org/10.1080/09593985.2017.1394411>.
54. Büyükturan Ö, Büyükturan B, Yetiş M, Yetiş A. Yaşlı bireylerde cilt yüzeyi üzerinden torasik kifoz ve lumbal lordoz açılarının değerlendirilmesi: spinal Mouse geçerliliği ve güvenilirliği. *Dicle Tıp Derg*. 2018;45:121–127. <https://doi.org/10.5798/dicletip.410864>.
55. de Oliveira TS, Candotti CT, La Torre M, Pelinson PPT, Furlanetto TS, Kutchak FM, et al. Validity and reproducibility of the measurements obtained using the flexicurve instrument to evaluate the angles of thoracic and lumbar curvatures of the spine in the sagittal plane. *Rehabil Res Pract*. 2012;1–9. <https://doi.org/10.1155/2012/186156>.
56. D'Osualdo F, Schierano S, Iannis M. Validation of clinical measurement of kyphosis with a simple instrument, the arcometer. *Spine (Phila Pa 1976)*. 1997;22:408–413. <https://doi.org/10.1097/00007632-1997022150-00011>.
57. Faramarzi Kohnesh Shahri Y, Ghani Zadeh Hesar NG. Validity and reliability of smartphonebased GoniometerPro app for measuring the thoracic kyphosis. *Musculoskelet Sci Pract*. 2020;49. <https://doi.org/10.1016/j.msksp.2020.102216>.
58. Giglio CA, Volpon JB. Development and evaluation of thoracic kyphosis and lumbar lordosis during growth. *J Child Orthop*. 2007;1:187–193. <https://doi.org/10.1007/s11832-007-0033-5>.
59. Gravina A, Ferraro C, Frizziero A, Ferraro M, Masiero S. Goniometer evaluation of thoracic kyphosis and lumbar lordosis in subjects during growth age: a validity study. *Stud, Health Technol Inform*. 2012;176:247–251. <https://doi.org/10.3233/978-1-61499-067-3-247>.
60. Grindle DM, Mousavi SJ, Allaire BT, White AP, Anderson DE. Validity of flexicurve and motion capture for measurements of thoracic kyphosis vs standing radiographic measurements. *JOR Spine*. 2020;3. <https://doi.org/10.1002/jsp2.1120>.
61. Hannink E, Dawes H, Shannon TML, Barker KL. Validity of sagittal thoracolumbar curvature measurement using a non-radiographic surface topography method. *Spine Deform*. 2022;10:1299–1306. <https://doi.org/10.1007/s43390-022-00538-0>.
62. Hunter DJ, Rivett DA, McKiernan S, Weerasekera I, Snodgrass SJ. Is the inclinometer a valid measure of thoracic kyphosis? A cross-sectional study. *Brazilian J Phys Ther*. 2018;22:310–317. <https://doi.org/10.1016/j.bjpt.2018.02.005>.
63. Sangtarash F. Validity and reliability of dual digital inclinometer in measuring thoracic kyphosis in women over 45 years. *J Spine*. 2013;3:1–4. <https://doi.org/10.4172/2165-7939.1000170>.
64. Schmidt AV, Andrade RM, Novo NF, Ribeiro AP. Revista medicina legal de costa rica. *Rev Med Leg Costa Rica*. 2022;39:74–75. <https://orcid.org/0000-0002-1061-3789>.
65. Sharifnezhad A, Raissi GR, Forogh B, Soleymanzadeh H, Mohammadpour S, Daliran M, Cham MB. The validity and reliability of Kinovea software in measuring thoracic kyphosis and lumbar lordosis. *Iran Rehabil J*. 2021;19:129–136. <https://doi.org/10.32598/IRJ.19.2.670.1>.
66. Spencer L, Fary R, McKenna L, Ho R, Briffa K. Thoracic kyphosis assessment in postmenopausal women: an examination of the Flexicurve method in comparison to radiological methods. *Osteoporos Int*. 2019;30:2009–2018. <https://doi.org/10.1007/s00198-019-05023-5>.
67. Tabard-Fougère A, Bonnefoy-Mazure A, Dhoubi A, Valaikaite R, Armand S, Dayer R. Radiation-free measurement tools to evaluate sagittal parameters in AIS patients: a reliability and validity study. *Eur Spine J*. 2019;28:536–543. <https://doi.org/10.1007/s00586-018-05875-1>.
68. Teixeira F, Carvalho G. Confiabilidade e validade das medidas da cifose torácica. *Rev Bras Fisioter*. 2007;11:199–204.
69. Todd C. Validation of spinal sagittal alignment with plain radiographs and the Debrunner kyphometer. *Med Res Arch*. 2015;2:1–25. <https://doi.org/10.18103/mra.v2i1.319>.
70. Tran TH, Wing D, Davis A, Bergstrom J, Schousboe JT, Nichols JF, et al. Correlations among four measures of thoracic kyphosis in older adults. *Osteoporos Int*. 2016;27: 1255–1259. <https://doi.org/10.1007/s00198-015-3368-7>.
71. Alderighi M, Ferrari R, Maghini I, Del Felice A, Masiero S. Intra and interrater reliability of spinal sagittal curves and mobility using pocket goniometer Inclimed® in healthy subjects. *J Back Musculoskelet Rehabil*. 2016;29:873–880. <https://doi.org/10.3233/BMR-160704>.
72. Amatachaya P, Wongsa S, Sooknuan T, Thaweewannakij T, Laophosri M, Manimanakorn N, et al. Validity and reliability of a thoracic kyphotic assessment tool measuring distance of the seventh cervical vertebra from the wall. *Hong Kong Physiother J*. 2016;35:30–36. <https://doi.org/10.1016/j.hkjp.2016.05.001>.
73. Barrett E, McCreesh K, Lewis J. Intrarater and interrater reliability of the flexicurve index, flexicurve angle, and manual inclinometer for the measurement of thoracic kyphosis. *Rehabil Res Pract*. 2013;2013:1–7. <https://doi.org/10.1155/2013/475870>.
74. Carvalho LACM, Aquino CF, Souza TR, Anjos MTS, Lima DBM, Fonseca ST. Clinical measures related to forward shoulder posture: a reliability and correlational study. *J Manipulative Physiol Ther*. 2019;42:141–147. <https://doi.org/10.1016/j.jmpt.2019.03.006>.
75. Demir E, Guzel NA, Kafa N. The reliability of measurements with the spinal mouse device in frontal and sagittal planes in asymptomatic female adolescents. *J Clin Anal Med*. 2019;1–4. <https://doi.org/10.4328/JCAM.6201>.

76. Devaney L, Bohannon R, Rizzo J, Capetta M, Vigneault J, Van Devere K. Inclino-metric measurement of kyphotic curvature: description and clinimetric properties. *Physiother Theory Pract*. 2017;33:797–804. <https://doi.org/10.1080/09593985.2017.1354950>.
77. Dunk NM, Lalonde J, Callaghan JP. Implications for the use of postural analysis as a clinical diagnostic tool: reliability of quantifying upright standing spinal postures from photographic images. *J Manip Physiol Ther*. 2005;28:386–392. <https://doi.org/10.1016/j.jmpt.2005.06.006>.
78. Elpeze G, Usgu G, Yigit S. Reliability of the smartphone application inclinometer and flexicurve in measuring thoracic kyphosis. *Cureus*. 2023. <https://doi.org/10.7759/cureus.35886>.
79. Gravina A, Ferraro C, Poli P, Barazzuol M, Del Felice A, Masiero S. Goniometric evaluation of the spinal sagittal curves in children and adolescents: a reliability study. *J Back Musculoskelet Rehabil*. 2017;30:325–331. <https://doi.org/10.3233/BMR-160541>.
80. Hannink E, Shannon T, Barker KL, Dawes H. The reliability and reproducibility of sagittal spinal curvature measurement using the Microsoft Kinect V2. *J Back Musculoskelet Rehabil*. 2019;33:295–301. <https://doi.org/10.3233/BMR-191554>.
81. MacIntyre NJ, Lorbergs AL, Adachi JD. Inclinometer-based measures of standing posture in older adults with low bone mass are reliable and associated with self-reported, but not performance-based, physical function. *Osteoporos Int*. 2014;25:721–728. <https://doi.org/10.1007/s00198-013-2484-5>.
82. Mannion AF, Knecht K, Balaban G, Dvorak J, Grob D. A new skin-surface device for measuring the curvature and global and segmental ranges of motion of the spine: reliability of measurements and comparison with data reviewed from the literature. *Eur Spine J*. 2004;13:122–136. <https://doi.org/10.1007/s00586-003-0618-8>.
83. Pakelöglu AC, Koç M, Yılmaz AS, Bayar B, Bayar K. Comparing the reliability of the Goniometer Pro application and flexicurve for measuring thoracic kyphosis: a cross-sectional study. *Int J Ther Rehabil*. 2023;30. <https://doi.org/10.12968/ijtr.2023.0013>.
84. Purser JL, Gold DT, McConnell ES, Schenkman MS, Morey MC, Branch LG, et al. Reliability of physical performance tests in four different randomized clinical trials. *Arch Phys Med Rehabil*. 1999;80:557–561. [https://doi.org/10.1016/S0003-9993\(99\)90199-5](https://doi.org/10.1016/S0003-9993(99)90199-5).
85. Twomey L, Raine S, Twomey L. Posture of the head, shoulders and thoracic spine in comfortable erect standing. *Aust J Physiother*. 1994;40:25–32. [https://doi.org/10.1016/S0004-9514\(14\)60451-7](https://doi.org/10.1016/S0004-9514(14)60451-7).
86. Roghani T, Khalkhali Zavieh M, Rahimi A, Talebian S, Manshadi FDehghan, et al. The reliability of standing sagittal measurements of spinal curvature and range of motion in older women with and without hyperkyphosis using a skin-surface device. *J Manip Physiol Ther*. 2017;40:685–691. <https://doi.org/10.1016/j.jmpt.2017.07.008>.
87. Saad KR, Colombo AS, Ribeiro AP, João SMA. Reliability of photogrammetry in the evaluation of the postural aspects of individuals with structural scoliosis. *J Bodyw Mov Ther*. 2012;16:210–216. <https://doi.org/10.1016/j.jbmt.2011.03.005>.
88. Şahinoğlu E, Ergin G, Bakırhan S, Ünver B. Reliability, concurrent validity, and minimal detectable change of a smartphone application for measuring thoracic kyphosis. *Clin Exp Heal Sci*. 2023;13 G:511–516. <https://doi.org/10.33808/clinephealthsci.1038122>.
89. Sedrez JA, Candotti CT, Rosa MIZ, Medeiros FS, Marques MT, Loss JF. Test-retest, inter- and intra-rater reliability of the flexicurve for evaluation of the spine in children. *Brazilian J Phys Ther*. 2016;20:142–147. <https://doi.org/10.1590/bjpt-rbf.2014.0139>.
90. Stolinski L, Kozinoga M, Czaprowski D, Tyrakowski M, Cerny P, Suzuki N, et al. Two-dimensional digital photography for child body posture evaluation: standardized technique, reliable parameters and normative data for age 7–10 years. *Scoliosis Spinal Disord*. 2017;12:38. <https://doi.org/10.1186/s13013-017-0146-7>.
91. Takatalo J, Ylinen J, Pienimäki T, Häkkinen A. Intra- and inter-rater reliability of thoracic spine mobility and posture assessments in subjects with thoracic spine pain. *BMC Musculoskelet Disord*. 2020;21. <https://doi.org/10.1186/s12891-020-03551-4>.
92. Temporiti F, Adamo P, Mandelli A, Buccolini F, Viola E, Aguzzi D, Gatti R, Barajon I. Test-retest reliability of a photographic marker-based system for postural examination. *Technol Heal Care*. 2023;31:1153–1160. <https://doi.org/10.3233/THC-220155>.
93. van Baalen GB, Vanwanseele B, Venter RR. Reliability and validity of a smartphone device and clinical tools for thoracic spine mobility assessments. *Sensors*. 2023;23. <https://doi.org/10.3390/s23177622>.
94. Van Blommestein AS, Lewis JS, Morrissey MC, Macrae S. Reliability of measuring thoracic kyphosis angle, lumbar lordosis angle and straight leg raise with an inclinometer. *The Open Spine J*. 2012;4:10–15. <https://doi.org/10.2174/1876532701204010010>.
95. Hinman MR. Interrater reliability of flexicurve postural measures among novice users. *J Back Musculoskelet Rehabil*. 2004;17:33–36. <https://doi.org/10.3233/BMR-2004-17107>.
96. Nair P, Bohannon RW, Devaney L, Maloney C, Romano A. Reliability and validity of nonradiologic measures of forward flexed posture in Parkinson disease. *Arch Phys Med Rehabil*. 2017;98:508–516. <https://doi.org/10.1016/j.apmr.2016.06.008>.
97. Cuijpers P, Griffin JW, Furukawa TA. The lack of statistical power of subgroup analyses in meta-analyses: a cautionary note. *Epidemiol Psychiatr Sci*. 2021;30(e78): 1–3. <https://doi.org/10.1017/S2045796021000664>.